

Ablation Methodology: Model Alpha M-14

One-component removal under the fixed evaluator.

full system 0.873 | calibration delta −0.031

Scope

Each condition removes one named component while retaining corpus, feature order, threshold, and score routine. The results are design-specific associations.

Interpretation


Calibration removal has the largest decrease; evidence normalization is next, while review routing is smaller but measurable.

Decision evidence

condition	macro F1	delta
full system	.873	baseline
no calibration	.842	−.031
no normalization	.851	−.022
no sequence order	.859	−.014
no review routing	.866	−.007

Component-delta bars

Topic-specific analytical figure for the same synthetic R184 record.

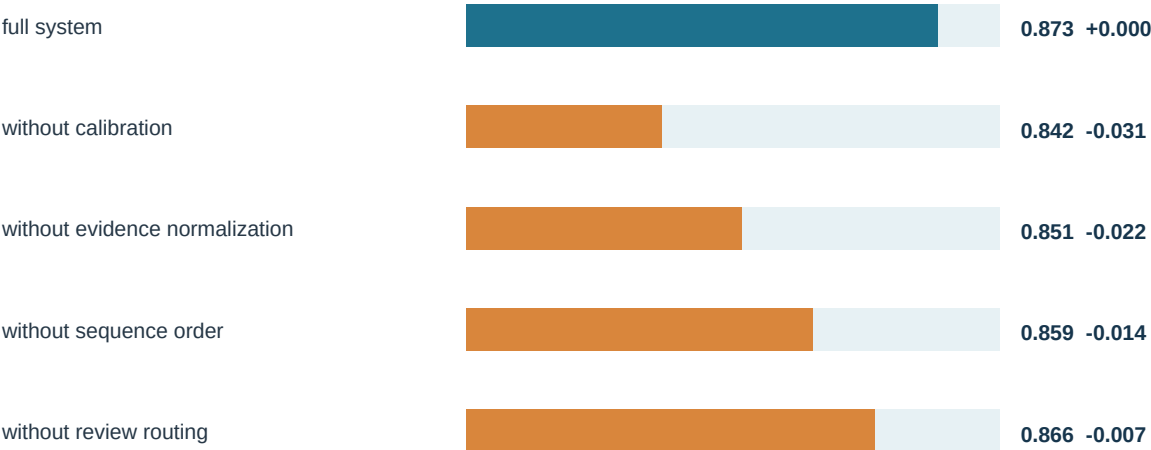

Interpretation:

Bar length encodes retained macro F1; annotations provide isolated deltas.