


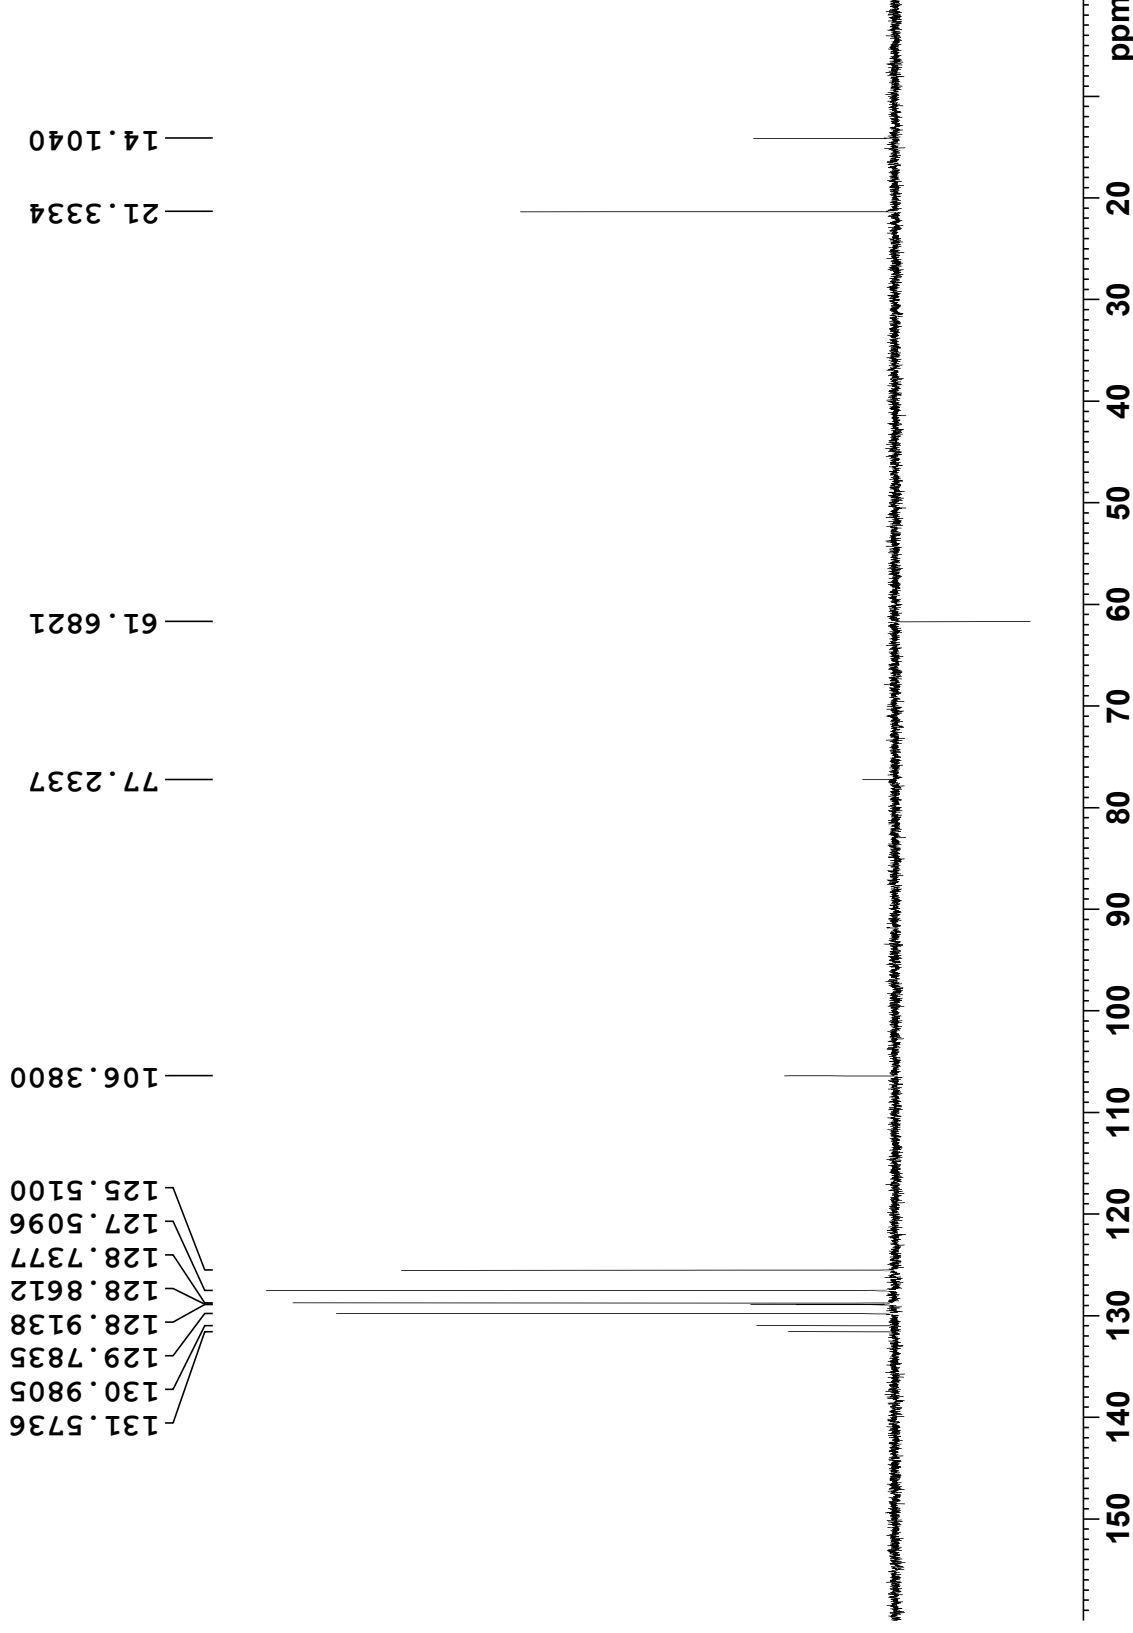

Current Data Parameters
NAME CLB
EXPNO 9
PROCNO 1

F2 - Acquisition Parameters

Date_ 20251219
Time_ 13.29 h
INSTRUM Avance
PROBHD Z151574_0199 (deptsp135
PULPROG 65536
TD 65536
SOLVENT CDCl3
NS 256
DS 8
SWH 30120.482 Hz
FIDRES 0.919204 Hz
AQ 1.0878977 sec
RG 101
DW 16.600 usec
DE 6.50 usec
TE 297.8 K
CNST2 145.0000000
D1 2.00000000 sec
D2 0.00344827 sec
D12 0.00002000 sec
TD0 1
SFO1 125.7703643 MHz
NUC1 13C
P1 9.00 usec
P13 2000.00 usec
PLW0 0 W
PLW1 96.00000000 W
SPNAM[5] Crp60comp.4
SPOAL5 0.500
SPOFFS5 0 Hz
SPW5 11.88099957 W
SFO2 500.1320005 MHz
NUC2 1H
CPDPRG2 A000
P3 8.00 usec
P4 16.00 usec
PCPD2 80.00 usec
PLW2 24.00000000 W
PLW12 0.23999999 W

F2 - Processing parameters

SI 32768
SF 125.7577885 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40