


Phi1 held-step map at first-NPBS D


forward: $V\lambda$ fit=0.7090 V, phase residual=0.231 rad

reverse: $V\lambda$ fit=0.7938 V, phase residual=0.223 rad


Held voltage-to-phase calibration

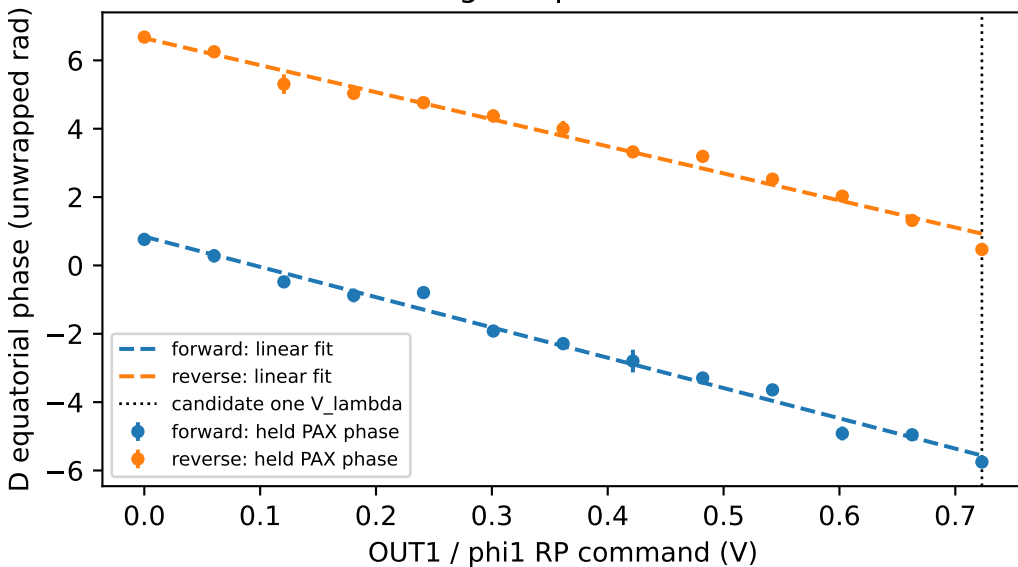

D-port equator check ($S_1 = 0$ ideal)

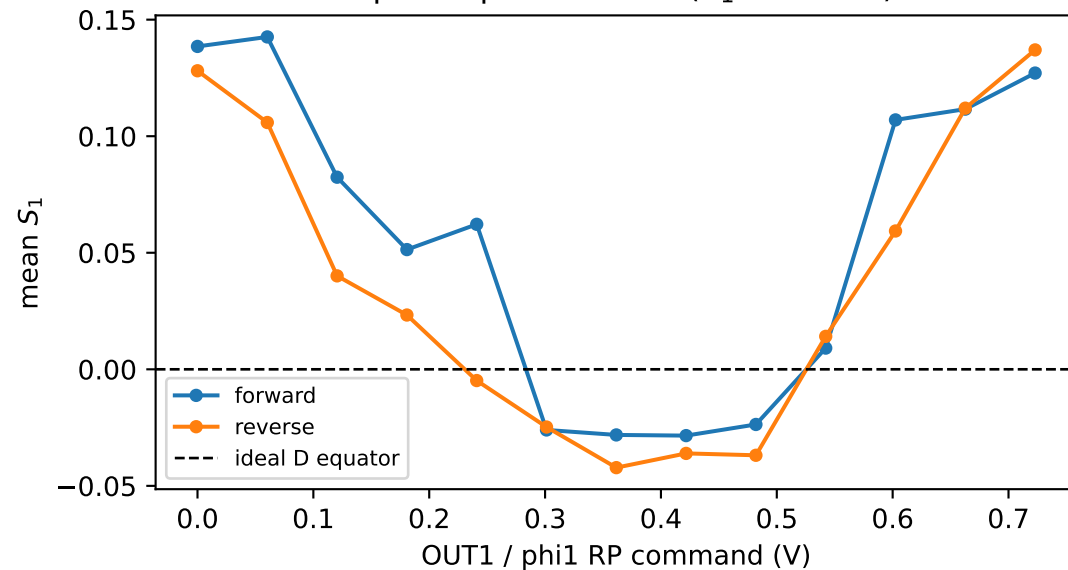

Held-step equatorial means

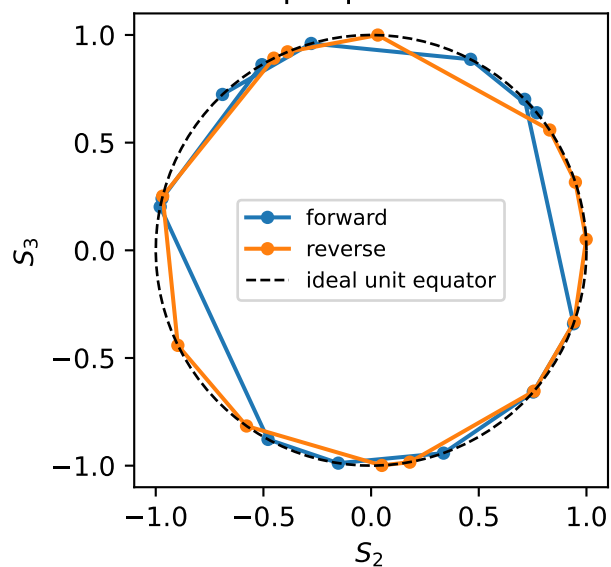

Simultaneous final-F PD monitor

