# PAX alignment run

## RUN

000620_pax-live_NPBS-reference-diagnostic_transmission-path
Status: completed

## ACQUISITION

Duration: 30.0 s; 155 fresh samples; 6.94 Hz over recorded samples.

## RUN COMMENT

simple T/R PAX measurement comparison. The first measurement corresponds to an unchanged PBS prepared polarization state seen through the reflected port of the NPBS in question, while the second measurement corresponds to the transmitted path.

## SETUP

In front of NPBS 1, C port
V_pi expectation only; verify channel and measured driver gain before calibration.

## DEFINITIONS

Power: watts. DoP: fraction. S1–S3: the suite's normalized direction (not multiplied by DoP). CSV theta/eta: radians; displayed angles: degrees. No fit or smoothing.

## RAW DATA

data.csv contains every accepted sample and the full exposed PAX record. Red Pitaya was not connected or measured. Settings/provenance: recipe.json and run.json.

## ACQUISITION ISSUES

None

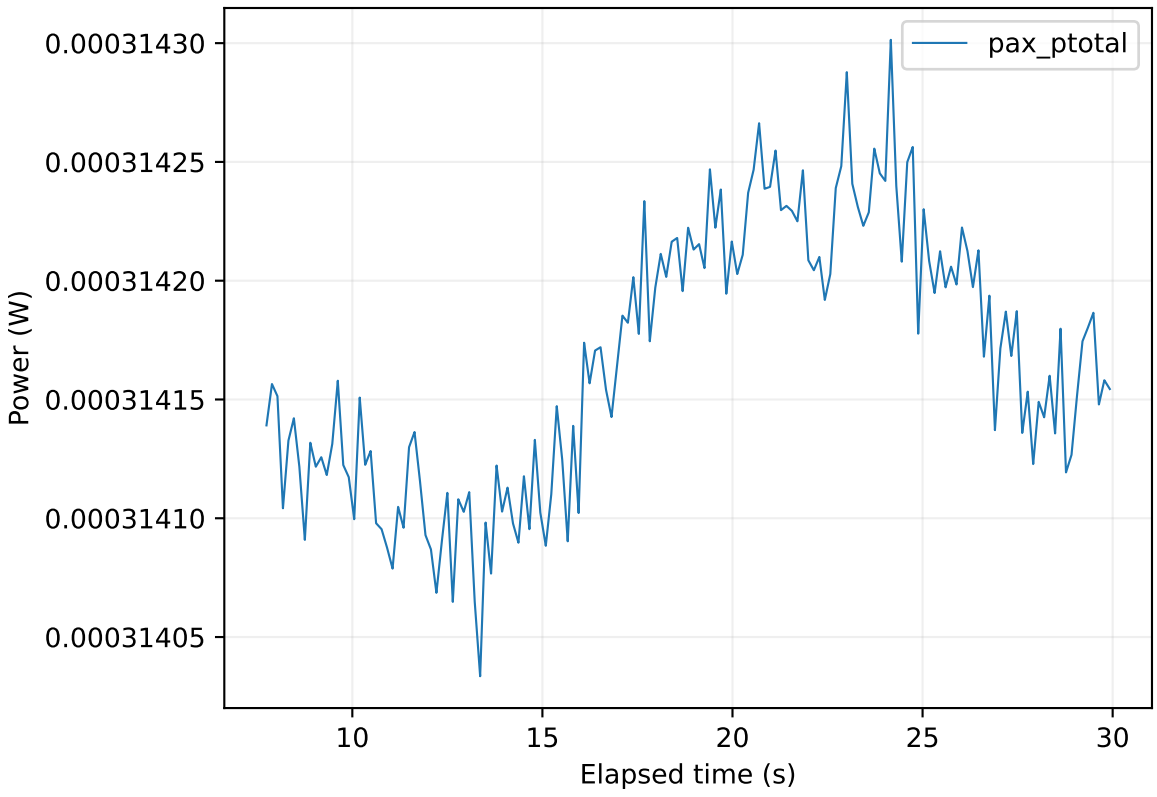
pax_ptotal
Power (W)
0.00031430
0.00031425
0.00031420
0.00031415
0.00031410
0.00031405
10
15
20
25
30
Elapsed time (s)

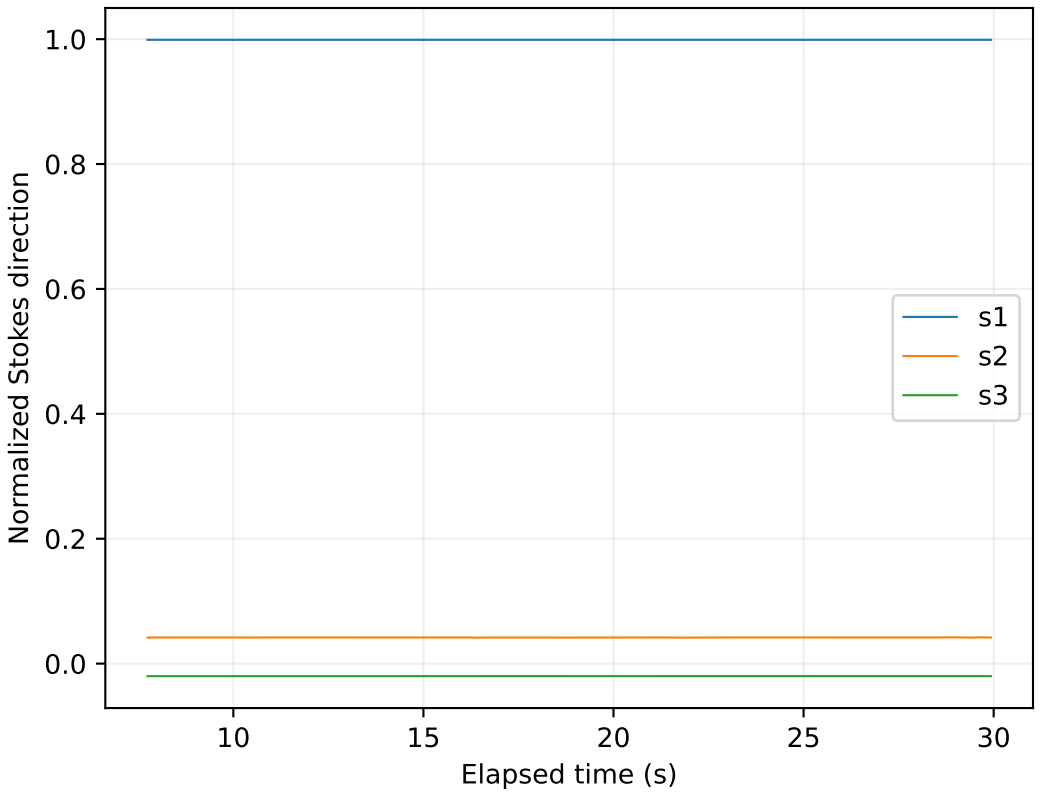
Normalized Stokes direction
1.0
0.8
0.6
0.4
0.2
0.0
s1
s2
s3
10
15
20
25
30
Elapsed time (s)

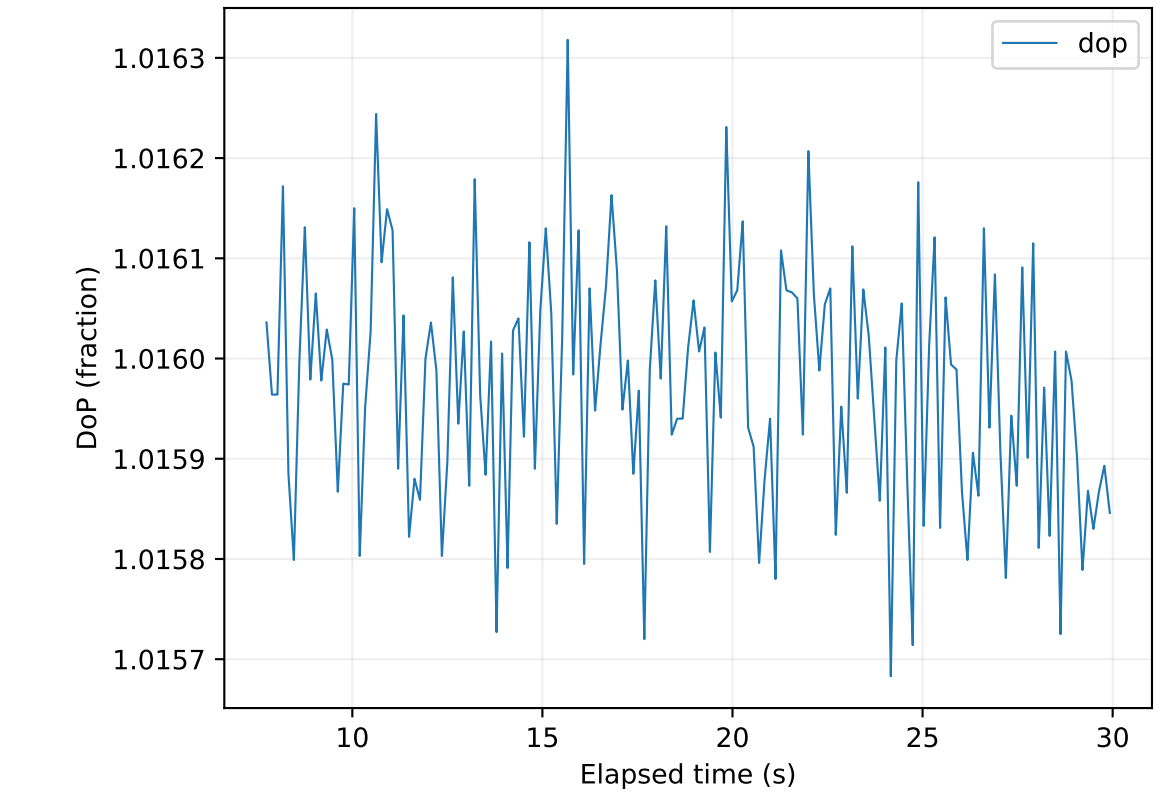
dop
DoP (fraction)
1.0163
1.0162
1.0161
1.0160
1.0159
1.0158
1.0157
10
15
20
25
30
Elapsed time (s)

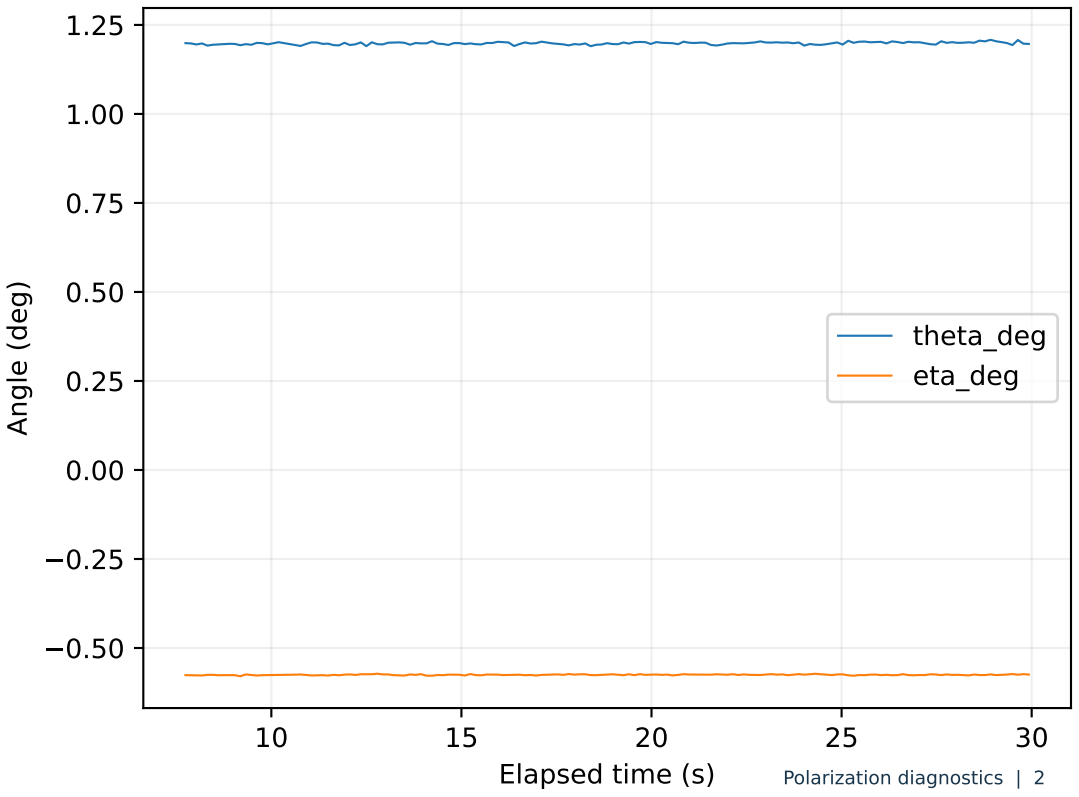
Angle (deg)
1.25
1.00
0.75
0.50
0.25
0.00
−0.25
−0.50
theta_deg
eta_deg
10
15
20
25
30
Elapsed time (s)