PAX alignment run

RUN

000951_pax-live_NPBS-reference-diagnostic_reflection-path
Status: completed

ACQUISITION

Duration: 30.2 s; 157 fresh samples; 6.94 Hz over recorded samples.

RUN COMMENT

same as last but reflected path

SETUP

In front of NPBS 1, C port
V_pi expectation only; verify channel and measured driver gain before calibration.

DEFINITIONS

Power: watts. DoP: fraction. S1–S3: the suite's normalized direction (not multiplied by DoP). CSV theta/eta: radians; displayed angles: degrees. No fit or smoothing.

RAW DATA

data.csv contains every accepted sample and the full exposed PAX record. Red Pitaya was not connected or measured. Settings/provenance: recipe.json and run.json.

ACQUISITION ISSUES

None

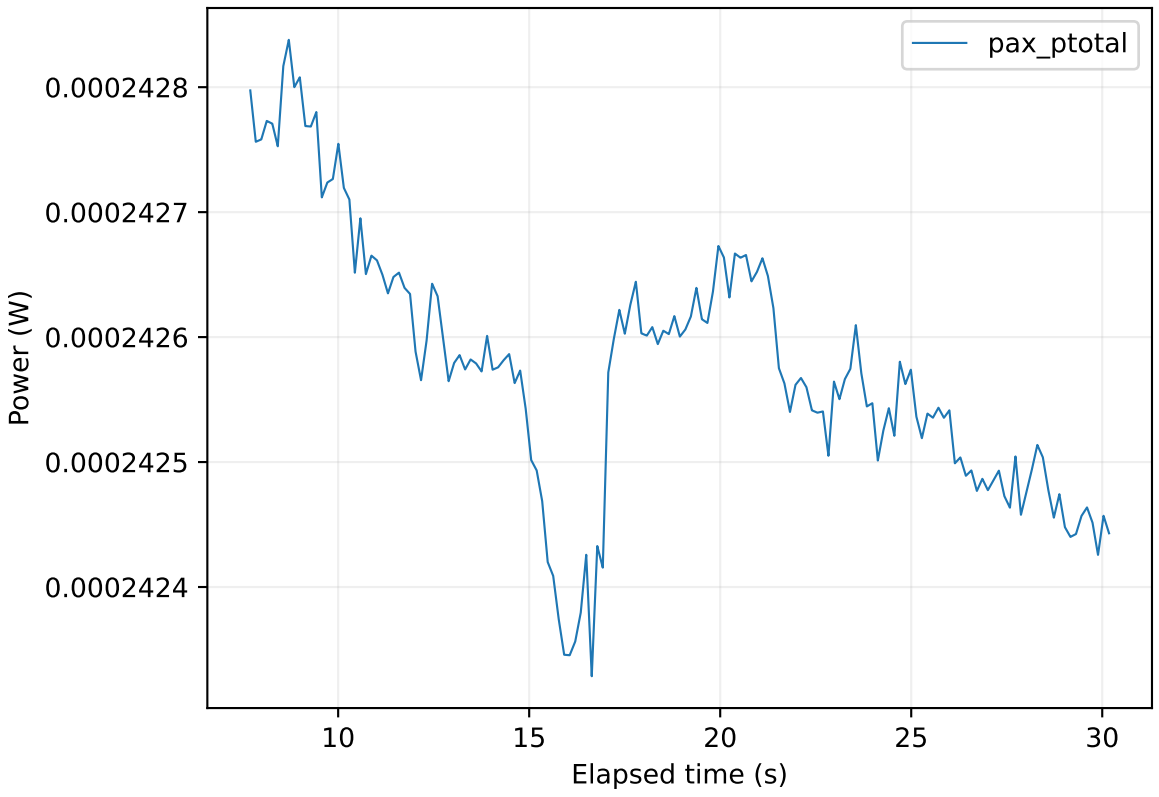
pax_ptotal
Power (W)
0.0002428
0.0002427
0.0002426
0.0002425
0.0002424
10
15
20
25
30
Elapsed time (s)

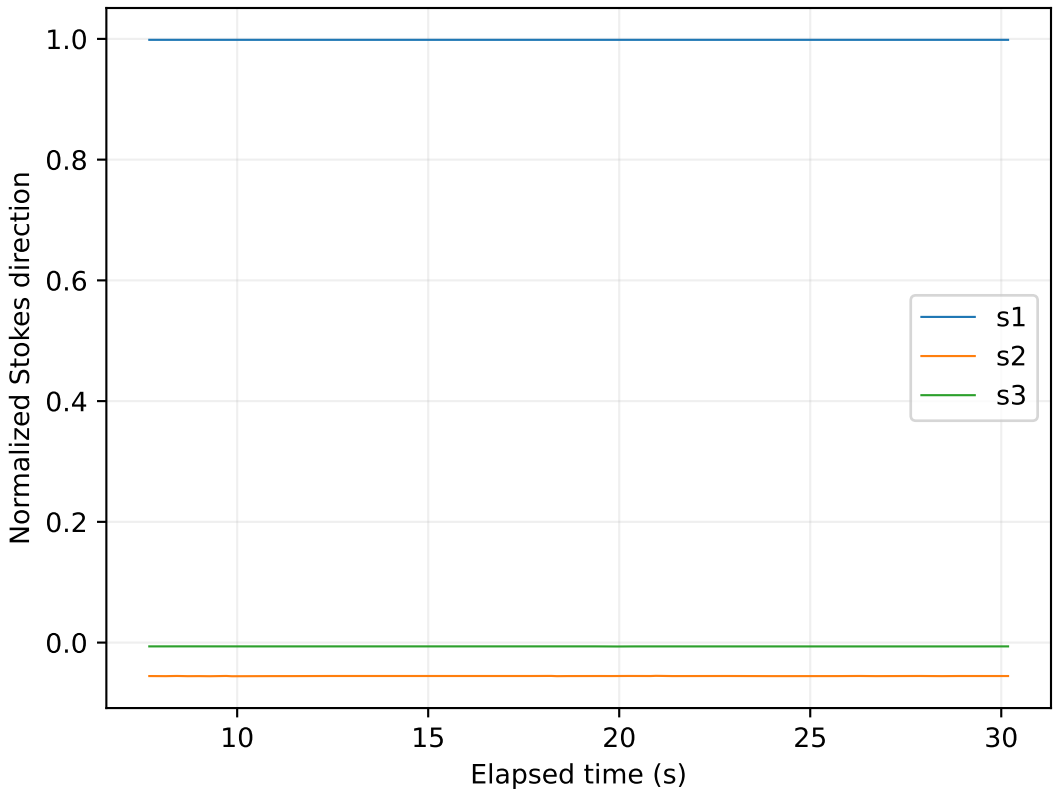
Normalized Stokes direction
1.0
0.8
0.6
0.4
0.2
0.0
s1
s2
s3
10
15
20
25
30
Elapsed time (s)

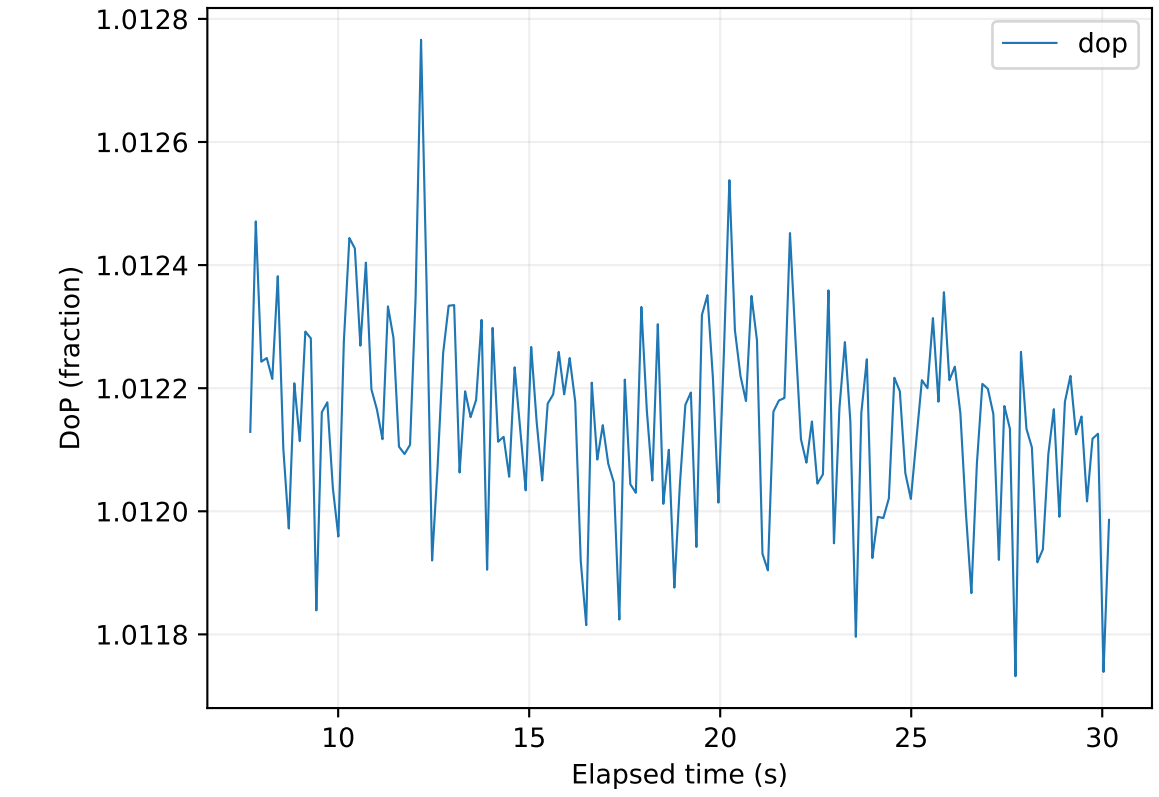
dop
DoP (fraction)
1.0128
1.0126
1.0124
1.0122
1.0120
1.0118
10
15
20
25
30
Elapsed time (s)

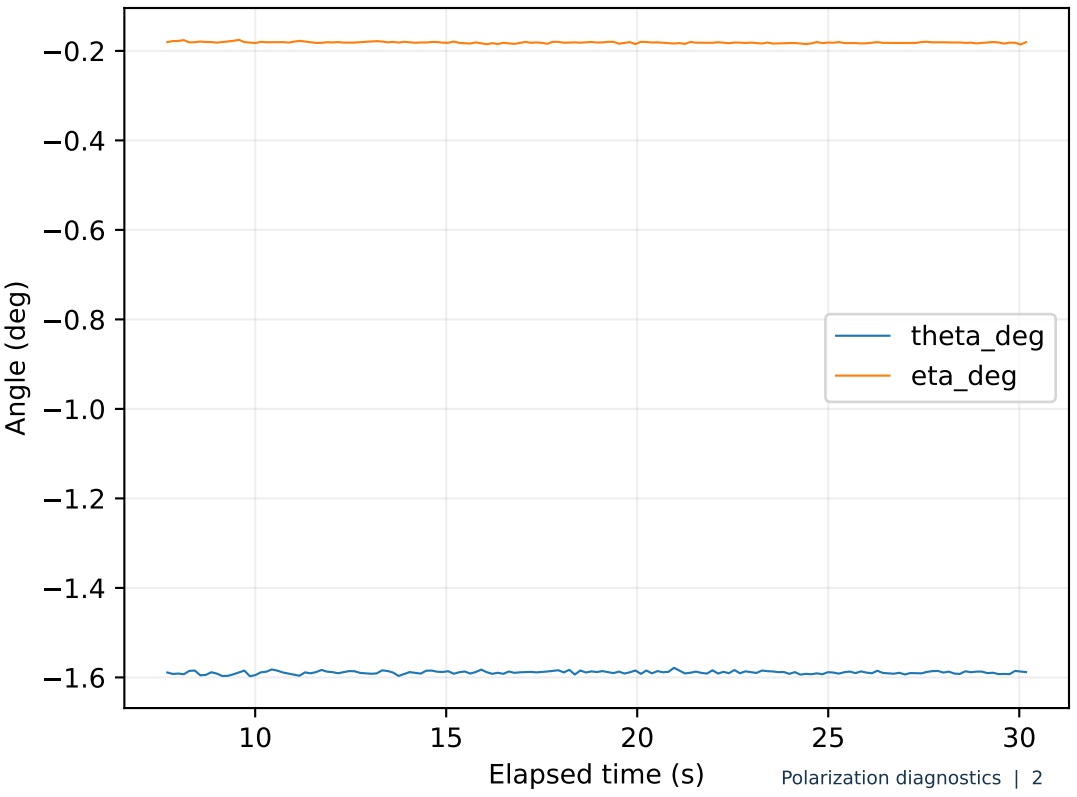
Angle (deg)
−0.2
−0.4
−0.6
−0.8
−1.0
−1.2
−1.4
−1.6
theta_deg
eta_deg
10
15
20
25
30
Elapsed time (s)