
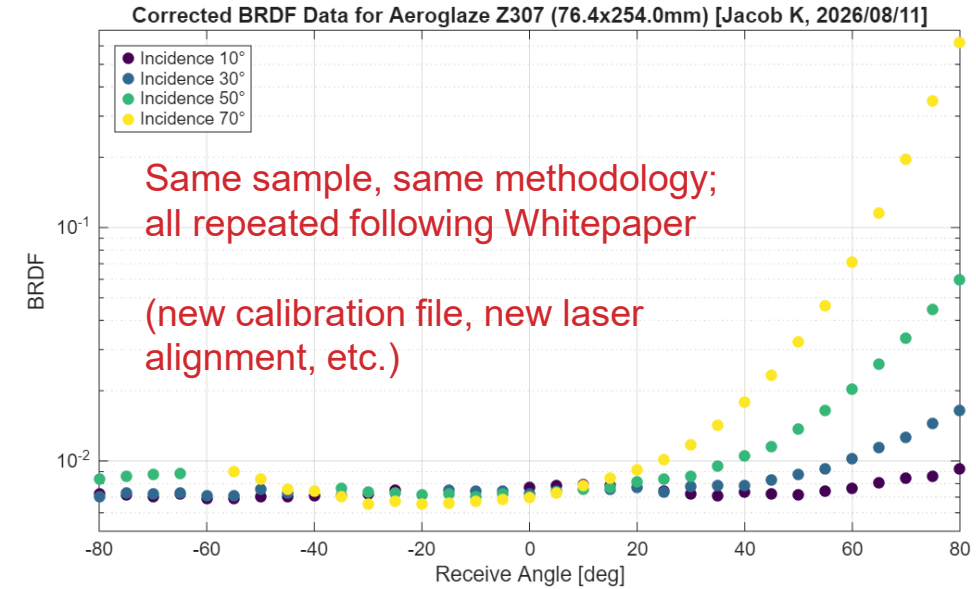


Comparison to Max's data

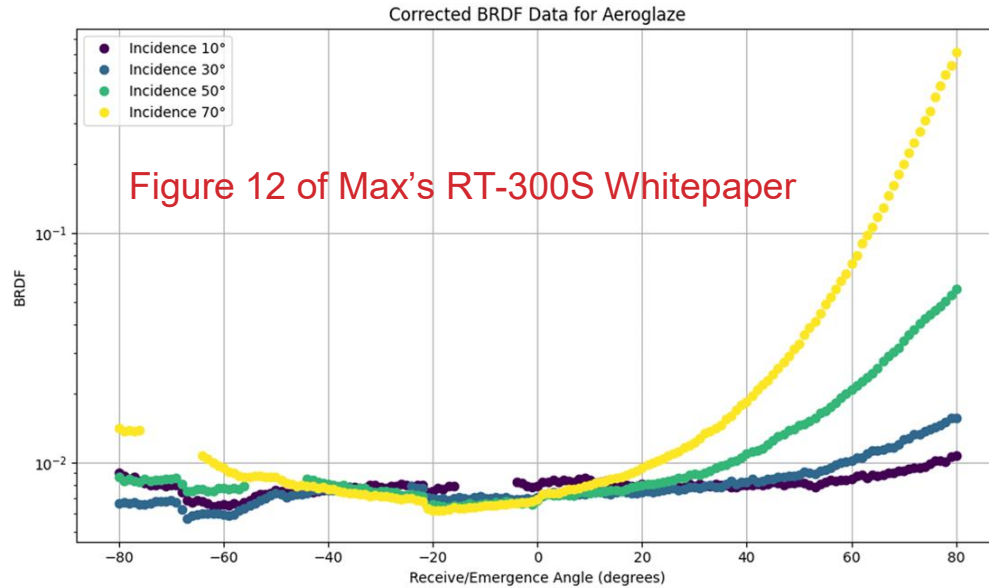

Conclusion

- RT-300S is calibrated according to prior methodology

Moving forward

- Fine-tune calibration/processing method
- Or look for other explanations (e.g., low angular sampling near specular... but seems unlikely to drive ~30% vs. ~6% TIS difference)

