

Heart Rhythm Assessment


Recorded on Feb 1, 2024 3:17 PM

Inconclusive

The ECG app can't classify this ECG reading.



Average
120 bpm

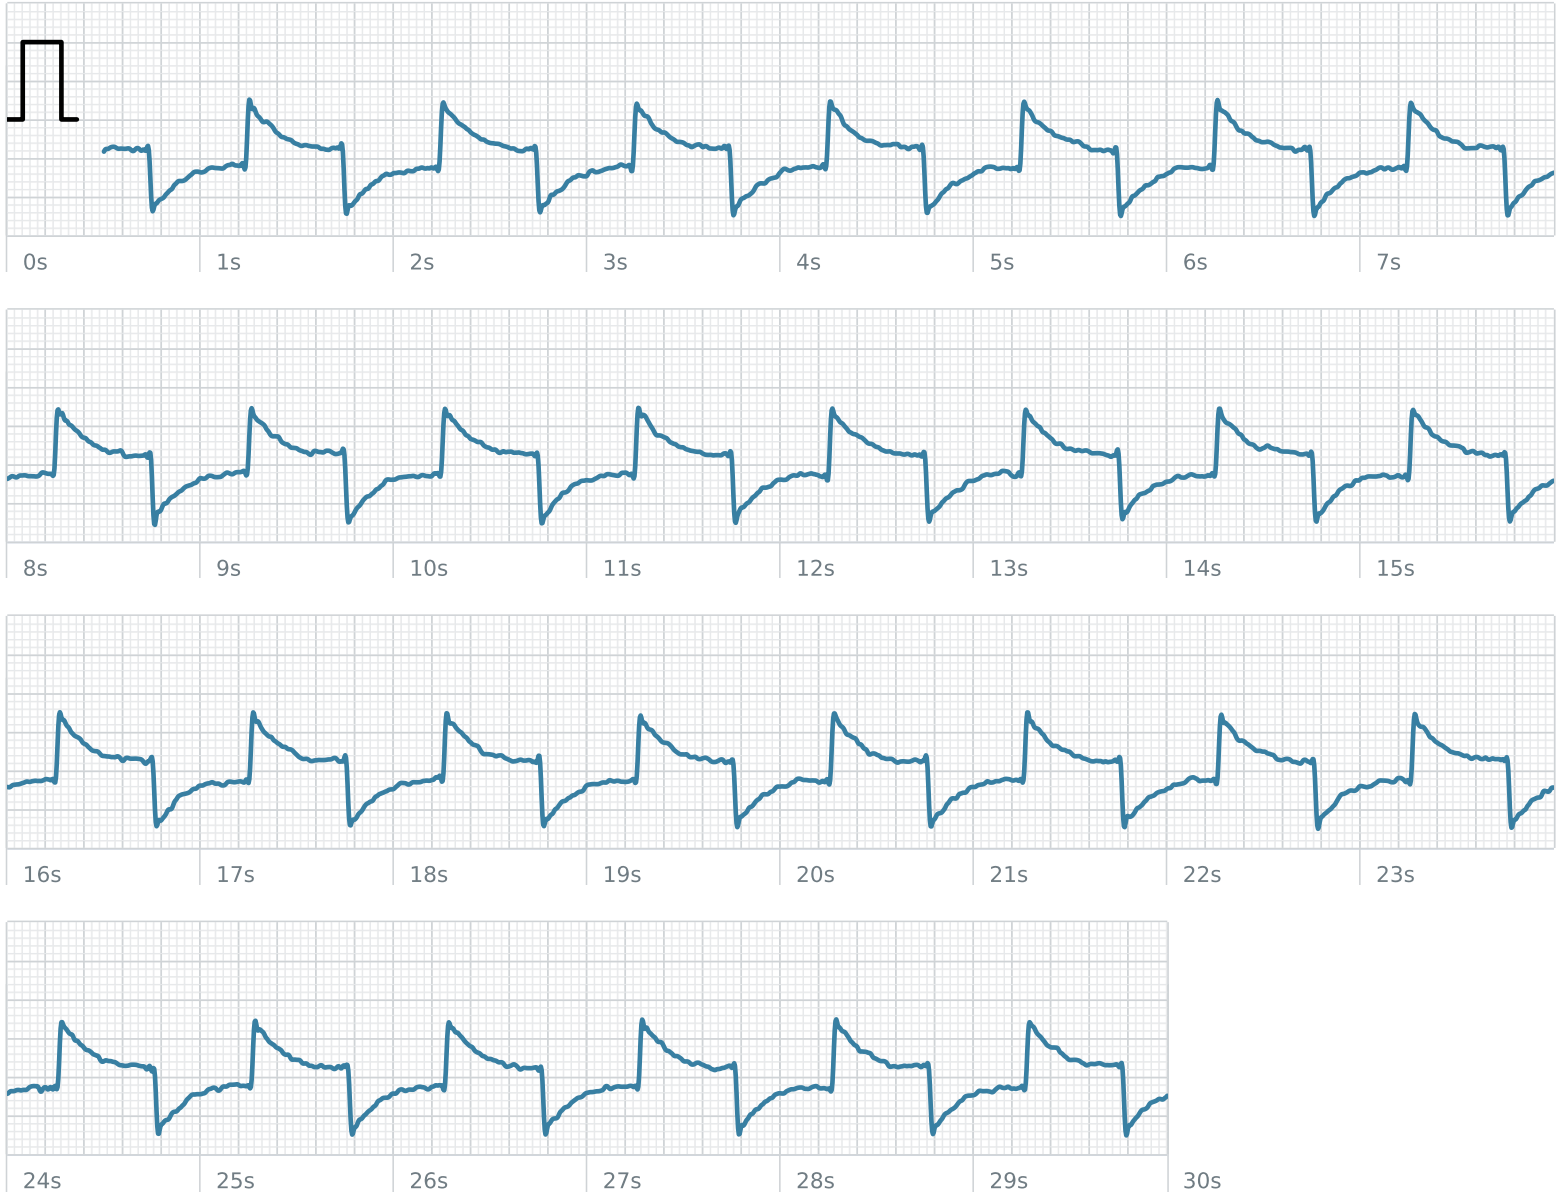

[25mm/s, 10mm/mV, 250 Hz] : [Qualitatively similar to a Lead I ECG]

About Fitbit's Heart Rhythm Assessment

How it works

We analyze data collected by the electrical sensors on your Fitbit device to determine if you have a normal sinus rhythm, an irregular heart rhythm suggestive of atrial fibrillation (AFib) or an inconclusive result.

Purpose & Performance

A convenient way to detect AFib. (This is not a diagnosis.) Our proprietary algorithm has been tested in a clinical study. (98.7% sensitivity, 100% specificity)