


Measurement: Voltage / Current

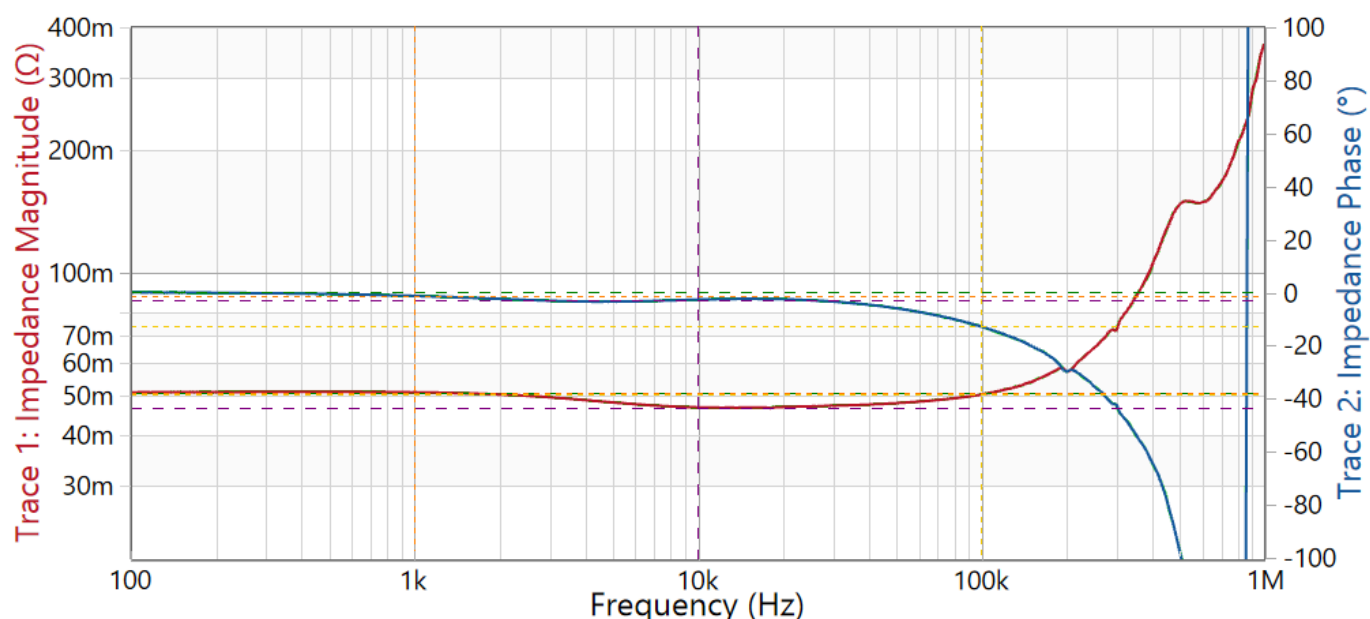

— Trace 1 — Trace 2 — ADC2 w/ inj. ... — ADC3 w/ inj. ...

	Cursor 1	Cursor 2	Cursor 3	Cursor 4
Frequency	100 Hz	1 kHz	10 kHz	100 kHz
Trace 1 Magnitude	50,925 mΩ	50,949 mΩ	46,791 mΩ	50,272 mΩ
Trace 2 Phase (°)	30,142 m°	-1,266 °	-2,642 °	-12,748 °

Hardware configuration	
Receiver bandwidth	300 Hz
Source level	5 dBm
DUT settling time	0 s
Sweep time	0 s

Termination	Channel 1	Channel 2
Impedance	1 MΩ	1 MΩ

Receiver switch	Receiver 1	Receiver 2
Impedance/Reflection	External	External

Attenuator setting	Receiver 1	Receiver 2
Impedance/Reflection	30 dB	10 dB

Shaped level	
Level	Constant

Device configuration	
Device type	Bode100R2
Serial number	PG276H
Last internal calibration	-

Sweep configuration	
Start frequency	100 Hz
Stop frequency	1 MHz
Center frequency	500,05 kHz
Span frequency	999,9 kHz
Sweep mode	Logarithmic
Number of points	300

Calibration/Correction	Full-Range	User-Range
Impedance	-	-