


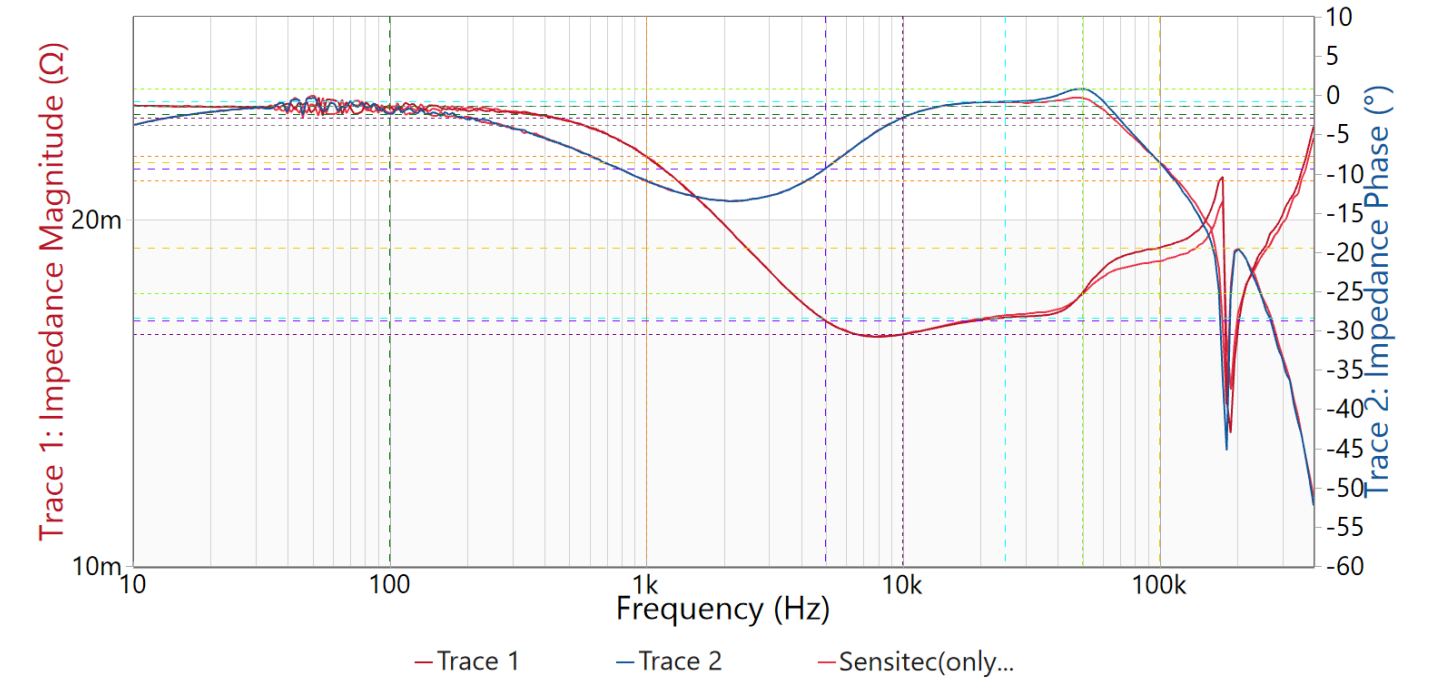

	Cursor 8	Cursor 1	Cursor 2	Cursor 6
Frequency	10 Hz	100 Hz	1 kHz	5 kHz
Trace 1 Magnitude	25,117 mΩ	25,123 mΩ	22,699 mΩ	16,326 mΩ
Trace 2 Phase (°)	-3,806 °	-2,395 °	-10,861 °	-9,333 °

	Cursor 3	Cursor 5	Cursor 7	Cursor 4
Frequency	10 kHz	25 kHz	50 kHz	100 kHz
Trace 1 Magnitude	15,888 mΩ	16,438 mΩ	17,251 mΩ	18,897 mΩ
Trace 2 Phase (°)	-2,866 °	-819,441 m°	791,385 m°	-8,508 °

Hardware configuration	
Receiver bandwidth	100 Hz
Source level	0 dBm
DUT settling time	0 s
Sweep time	22,37 s

Device configuration	
Device type	Bode100R2
Serial number	PG276H
Last internal calibration	01/16/2025 14:34:34

Termination	Channel 1	Channel 2
Impedance	1 MΩ	1 MΩ

Sweep configuration	
Start frequency	10 Hz
Stop frequency	400 kHz
Center frequency	200,005 kHz
Span frequency	399,99 kHz
Sweep mode	Logarithmic
Number of points	300

Receiver switch	Receiver 1	Receiver 2
Impedance/Reflection	External	External

Attenuator setting	Receiver 1	Receiver 2
Impedance/Reflection	30 dB	0 dB

Calibration/Correction	Full-Range	User-Range
Impedance	-	-

Shaped level	
Level	Constant