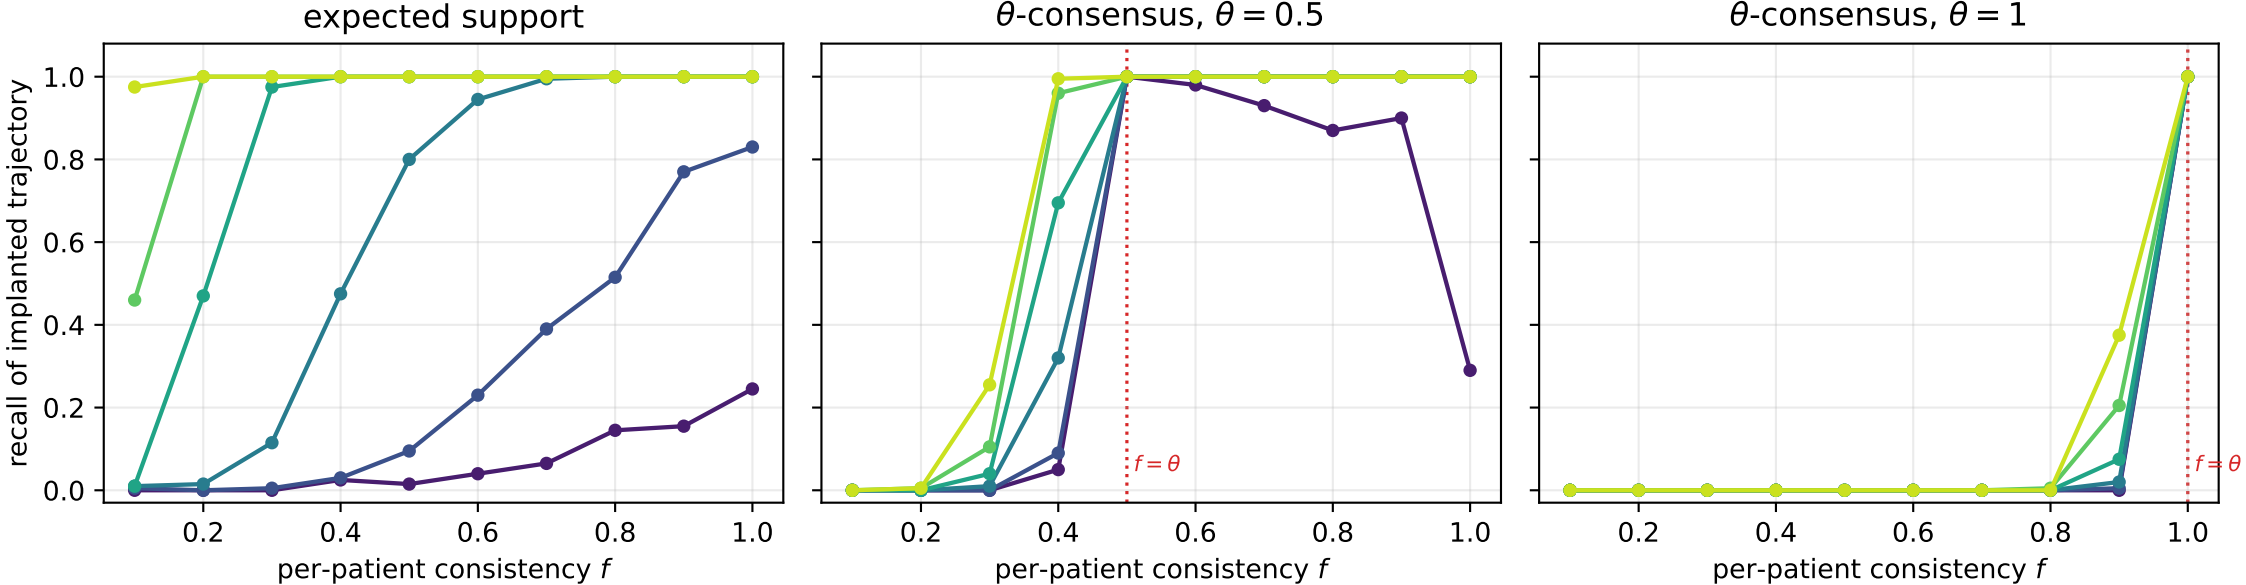
expected support
θ-consensus, θ = 0.5
θ-consensus, θ = 1
recall of implanted trajectory
per-patient consistency f
per-patient consistency f
per-patient consistency f
f = θ
f = θ
0.0
0.2
0.4
0.6
0.8
1.0
0.2
0.4
0.6
0.8
1.0
N=2
N=3
N=5
N=10
N=20
N=30