$\Sigma = 1:1$ Self-Reference Loop

The measurement apparatus IS the measured system

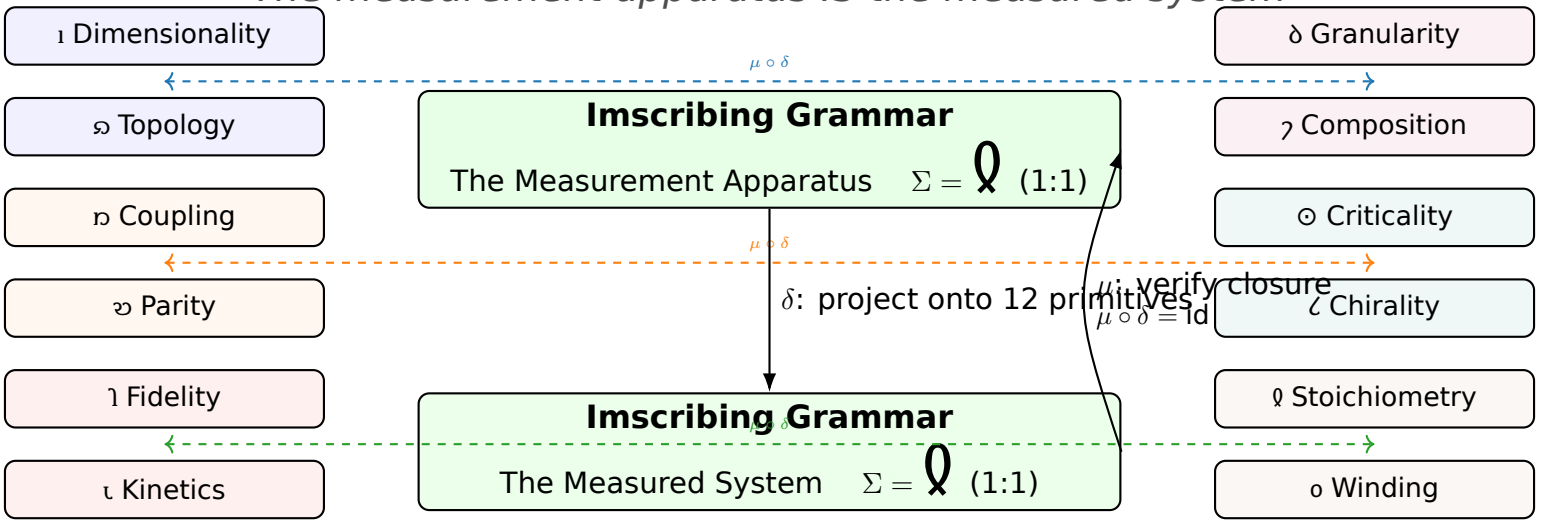

Why $\Sigma = 1:1$ is the key: In a conventional SIC-POVM, the dual basis $\tilde{\Pi}_i = d \cdot \Pi_i$ is a *distinct* set of operators. In the Grammar, $\mu \circ \delta = \text{id}$ means the verification pathway is encoded in the structure itself — no separate dual basis needed. $\Sigma = 1:1$ collapses apparatus and system into a single self-referential identity.