



Systemvergleich - Drucksensor (Baumer PP20H, 4-20 mA, 0-1 bar)
Messung 1: Derselbe Sensor (Atmosphaerendruck Berlin ~1026 hPa)
Messung 2: Anderer PP20H bereits installiert in der Anlage - Geblaease aktiv

M1 - Zeitverlauf (Atmosphaerendruck)

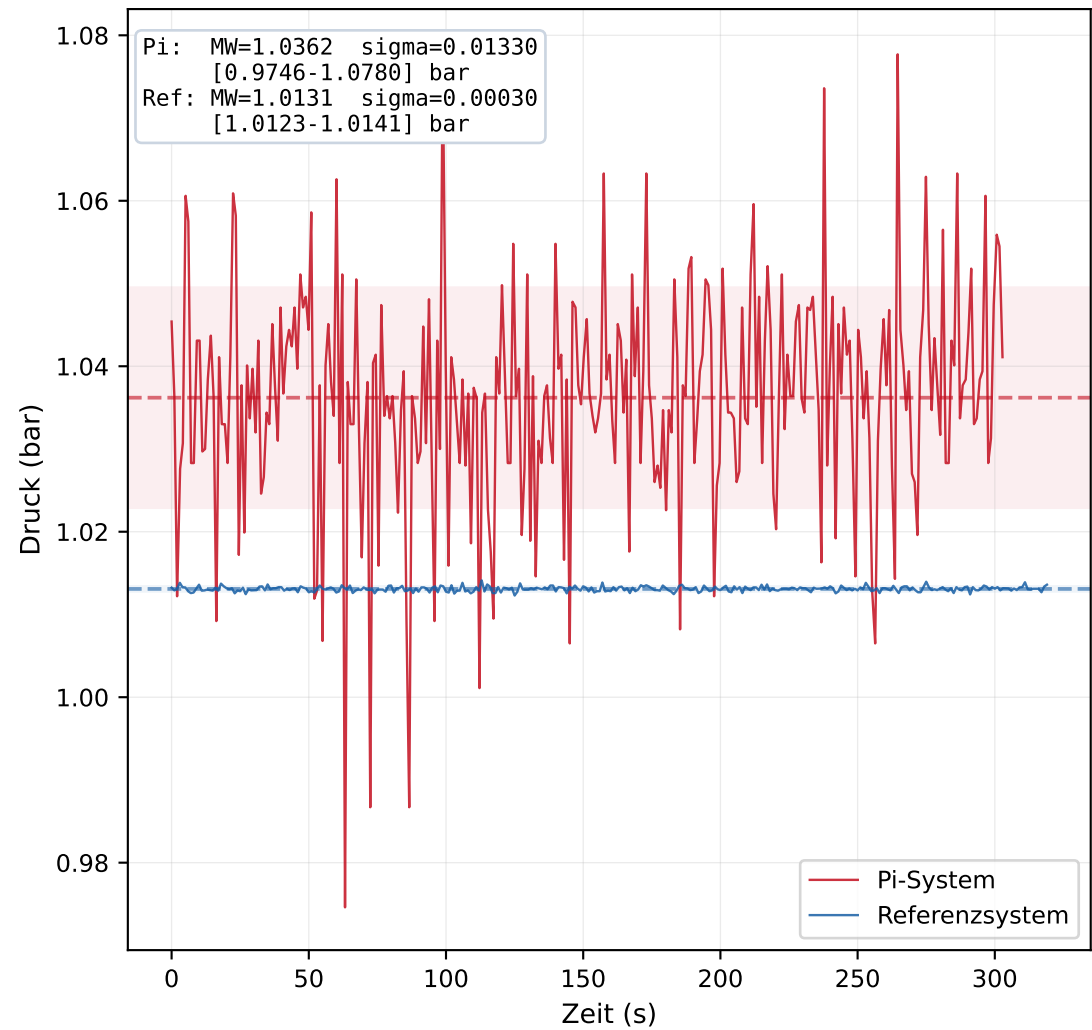

M1 - Verteilung (Atmosphaerendruck)

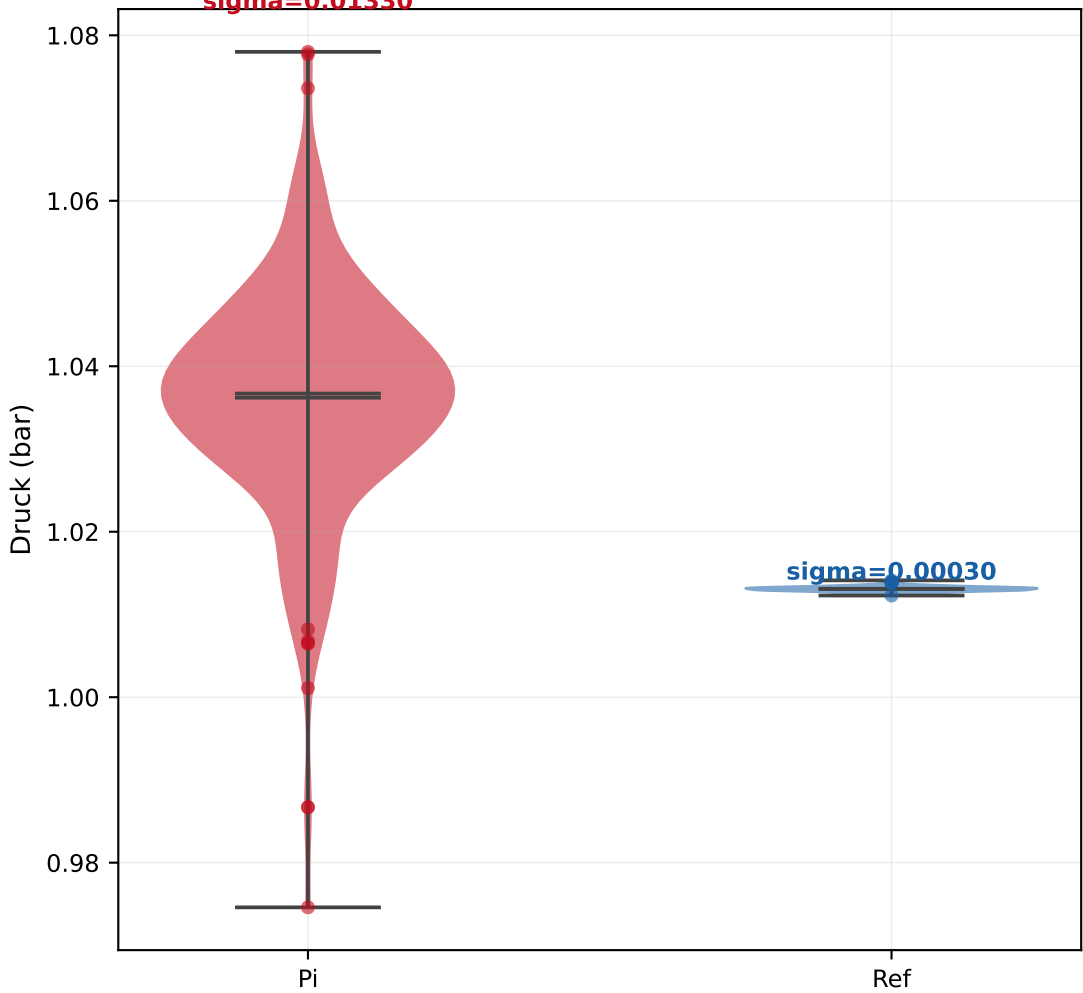


Statistische Auswertung
Druck



Metrik	Pi M1	Ref M1	Pi M2	Ref M2
MW (bar)	1.0362	1.0131	1.0481	1.0258
MW (mbar)	1036.2	1013.1	1048.1	1025.8
sigma (mbar)	13.30	0.30	14.02	0.86
Min (bar)	0.9746	1.0123	1.0078	1.0237
Max (bar)	1.0780	1.0141	1.0941	1.0306
Delta MW	-	23.1mbar	-	22.3mbar
sigma-Fakt.	-	44.7x	-	16.2x

M2 - Zeitverlauf (Geblaease aktiv)

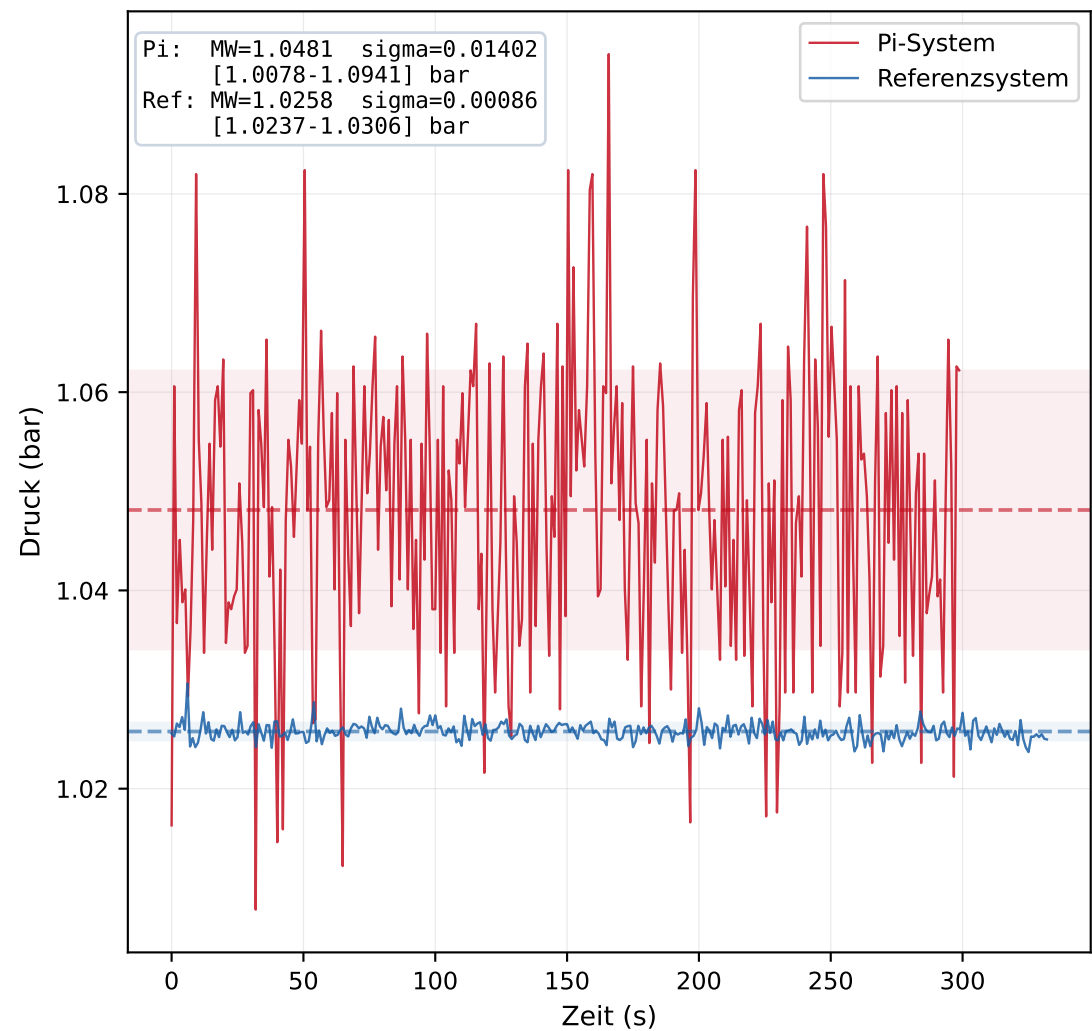

M2 - Verteilung (Geblaease aktiv)

