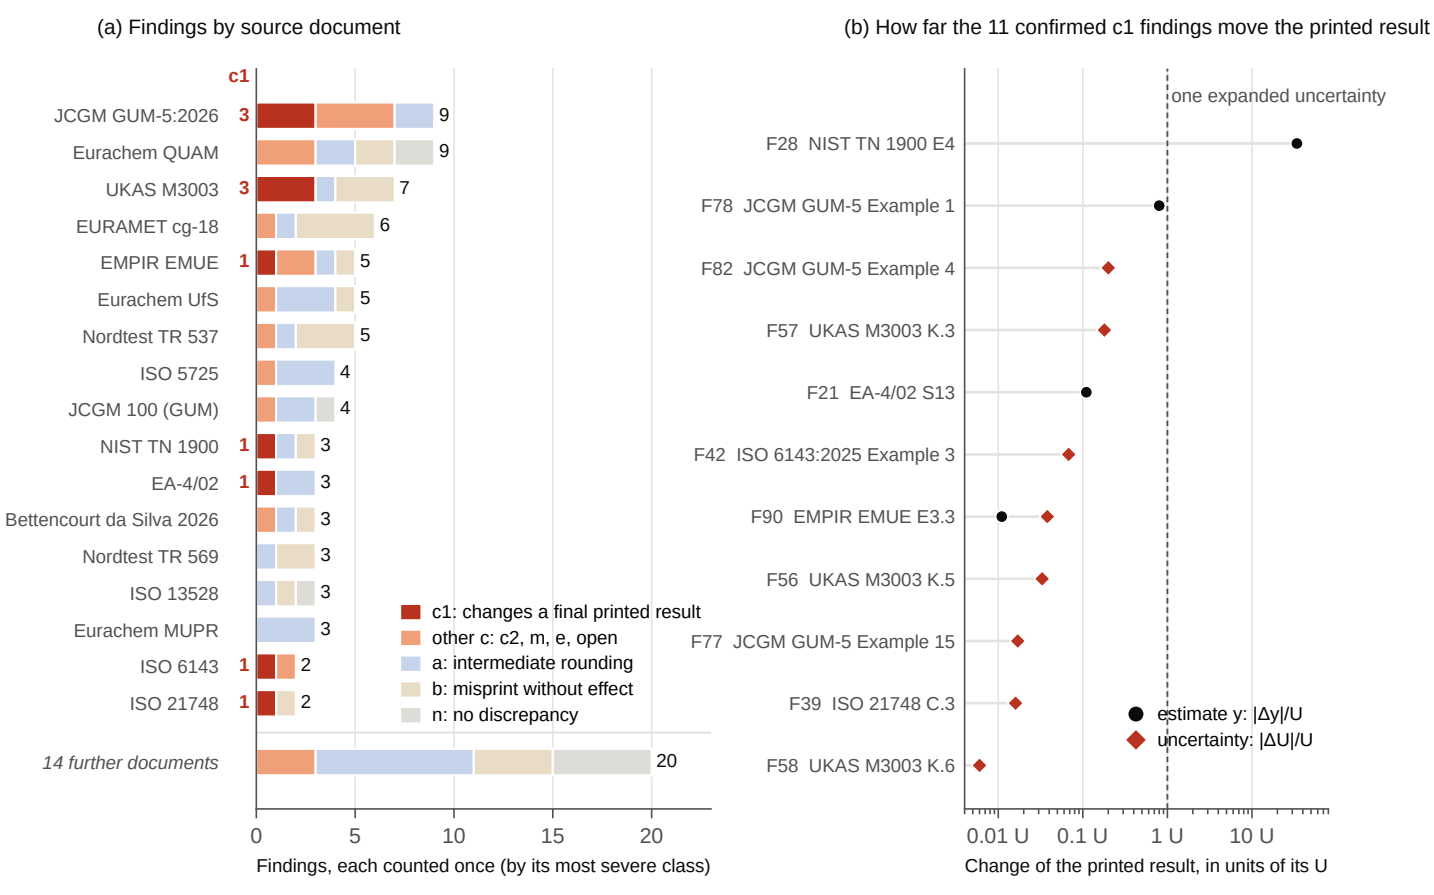
(a) Findings by source document
c1
JCGM GUM-5:2026 3 9
Eurachem QUAM 9
UKAS M3003 3 7
EURAMET cg-18 6
EMPIR EMUE 1 5
Eurachem UfS 5
Nordtest TR 537 5
ISO 5725 4
JCGM 100 (GUM) 4
NIST TN 1900 1 3
EA-4/02 1 3
Bettencourt da Silva 2026 3
Nordtest TR 569 3
ISO 13528 3
Eurachem MUPR 3
ISO 6143 1 2
ISO 21748 1 2
14 further documents 20
c1: changes a final printed result
other c: c2, m, e, open
a: intermediate rounding
b: misprint without effect
n: no discrepancy
0 5 10 15 20
Findings, each counted once (by its most severe class)
(b) How far the 11 confirmed c1 findings move the printed result
one expanded uncertainty
F28 NIST TN 1900 E4
F78 JCGM GUM-5 Example 1
F82 JCGM GUM-5 Example 4
F57 UKAS M3003 K.3
F21 EA-4/02 S13
F42 ISO 6143:2025 Example 3
F90 EMPIR EMUE E3.3
F56 UKAS M3003 K.5
F77 JCGM GUM-5 Example 15
F39 ISO 21748 C.3
F58 UKAS M3003 K.6
estimate y: |Δy|/U
uncertainty: |ΔU|/U
0.01 U 0.1 U 1 U 10 U
Change of the printed result, in units of its U