


Acetonitrile: calibration controls the result



20 s, residual standard deviation 0.001 dB

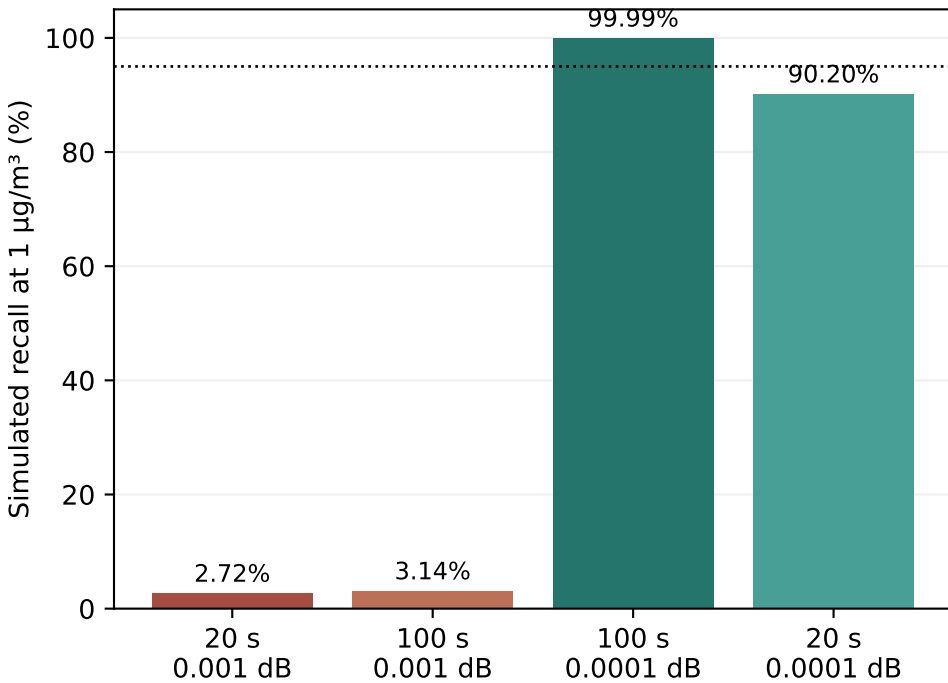