IP-13　Error code 32 (pg 1 of 1)
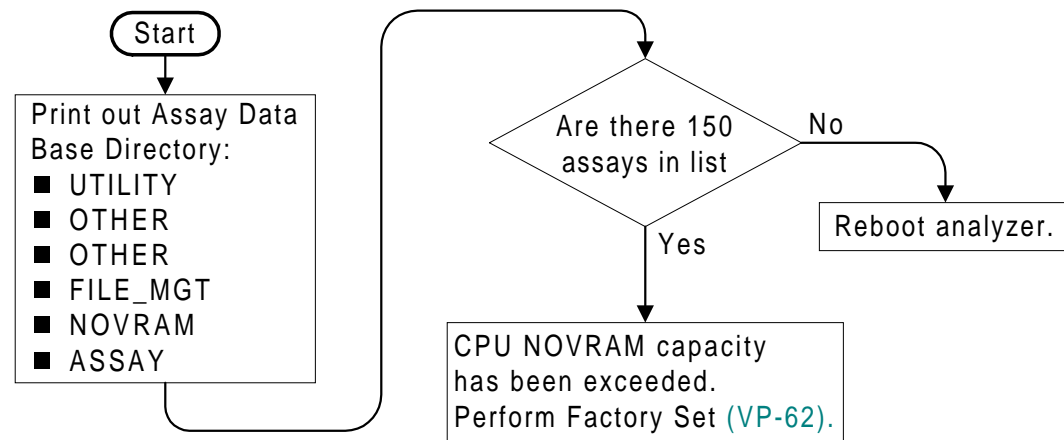EC-32: NOVRAM full

Start

Print out Assay Data
Base Directory:
■ UTILITY
■ OTHER
■ OTHER
■ FILE_MGT
■ NOVRAM
■ ASSAY

Are there 150 assays in list

No

Yes

Reboot analyzer.

CPU NOVRAM capacity
has been exceeded.
Perform Factory Set (VP-62).

IP13.vsd

| Chapter Contents | Manual Contents | CD Main Screen | Index |