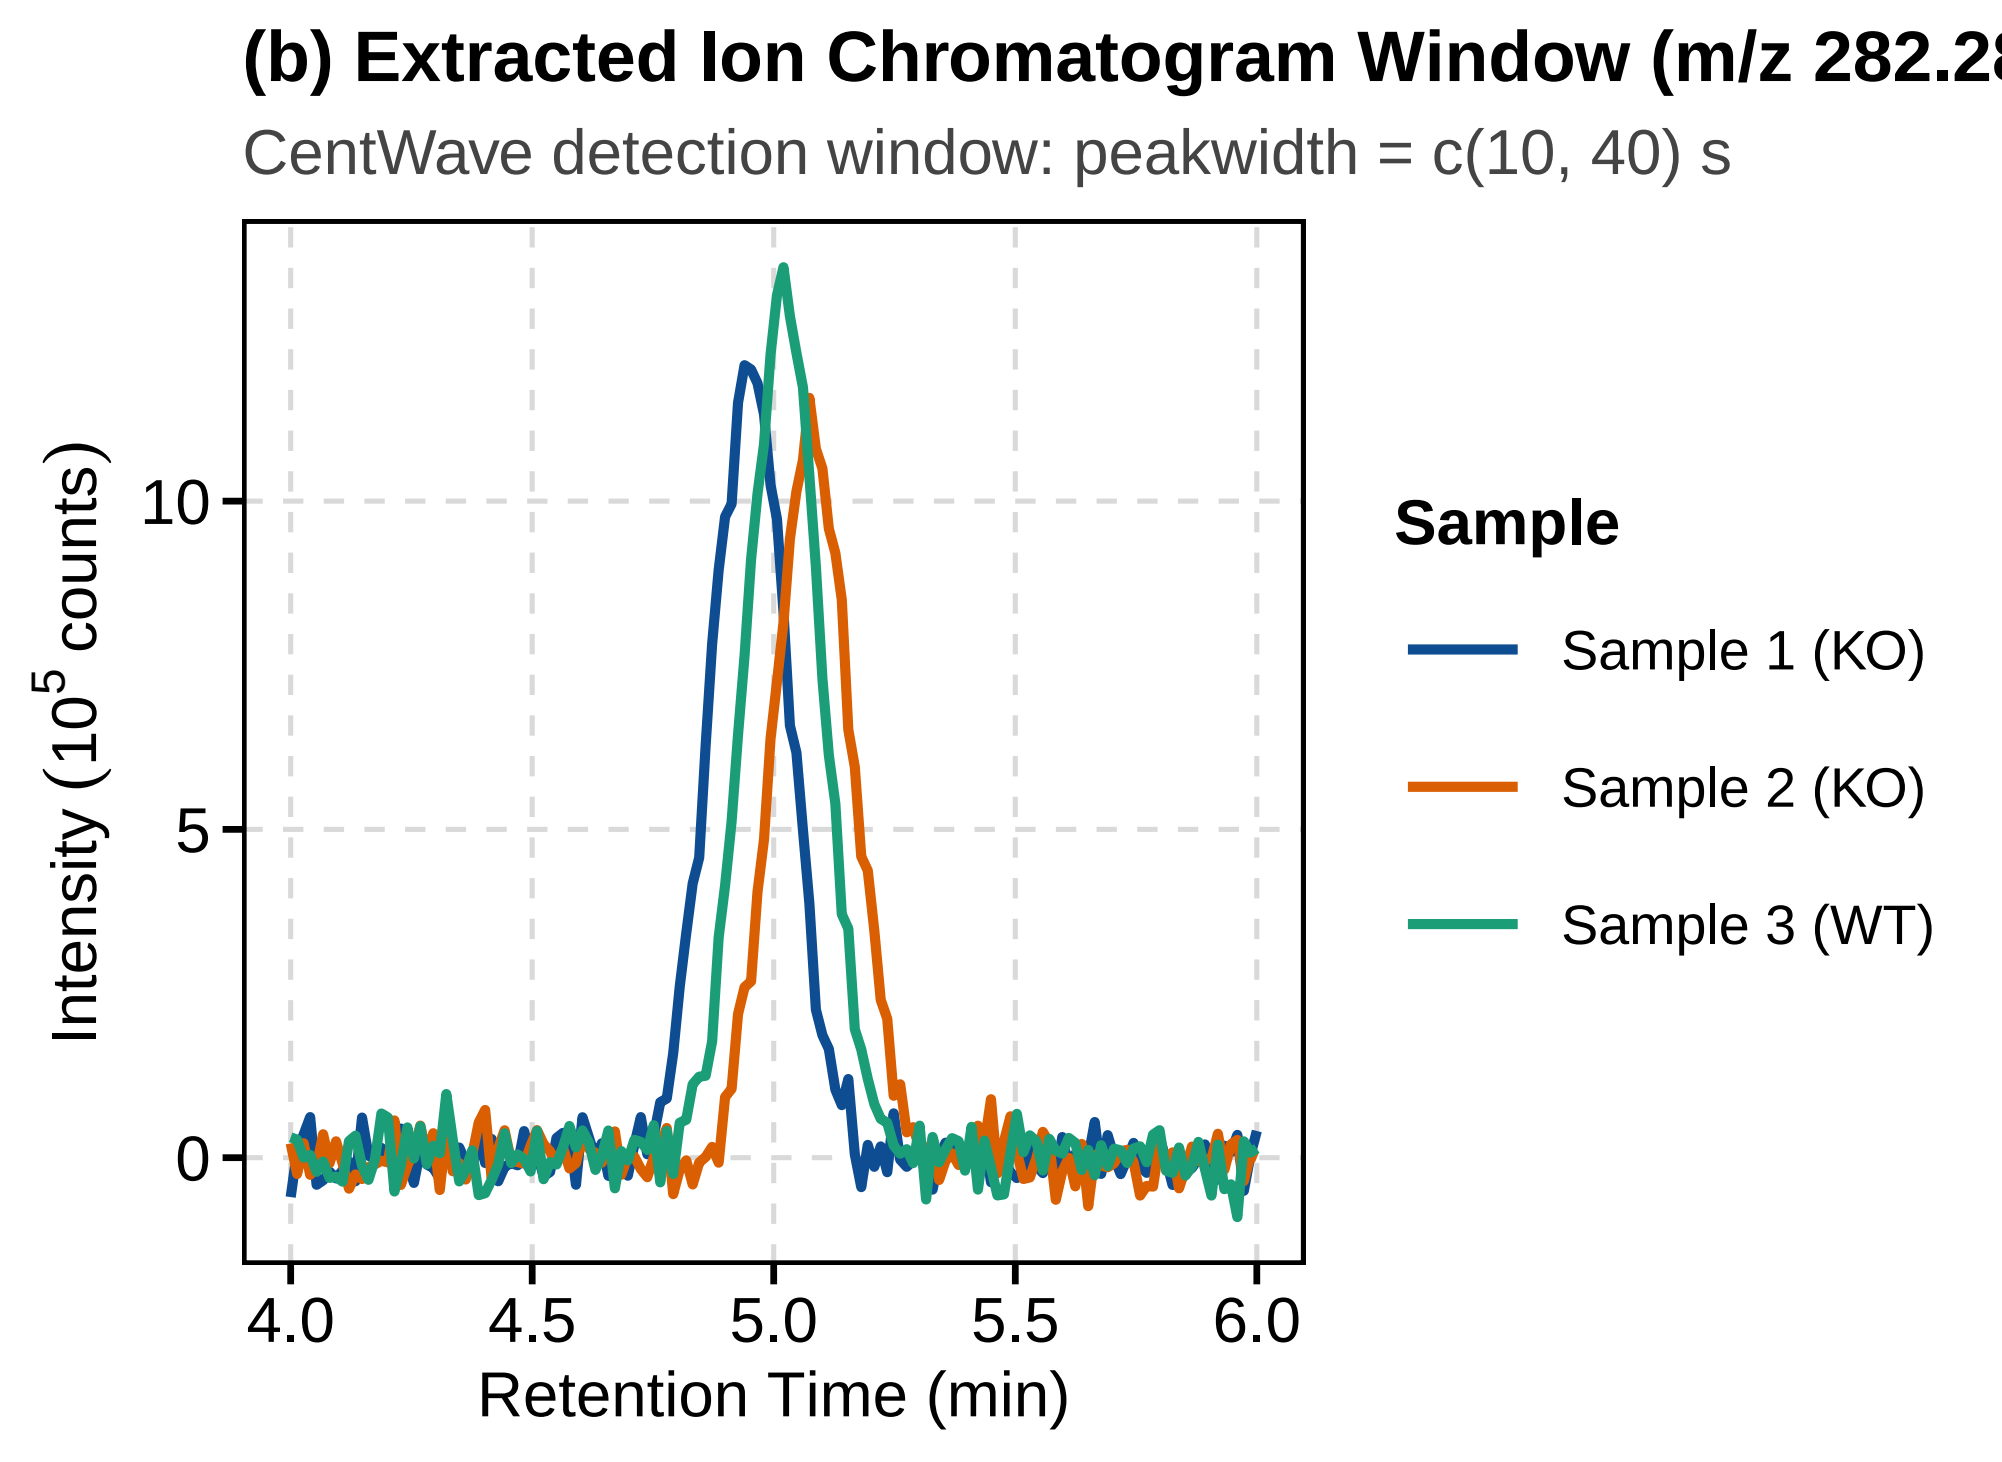
(b) Extracted Ion Chromatogram Window (m/z 282.28
CentWave detection window: peakwidth = c(10, 40) s
Intensity (10^5 counts)
10
5
0
4.0
4.5
5.0
5.5
6.0
Retention Time (min)
Sample
Sample 1 (KO)
Sample 2 (KO)
Sample 3 (WT)