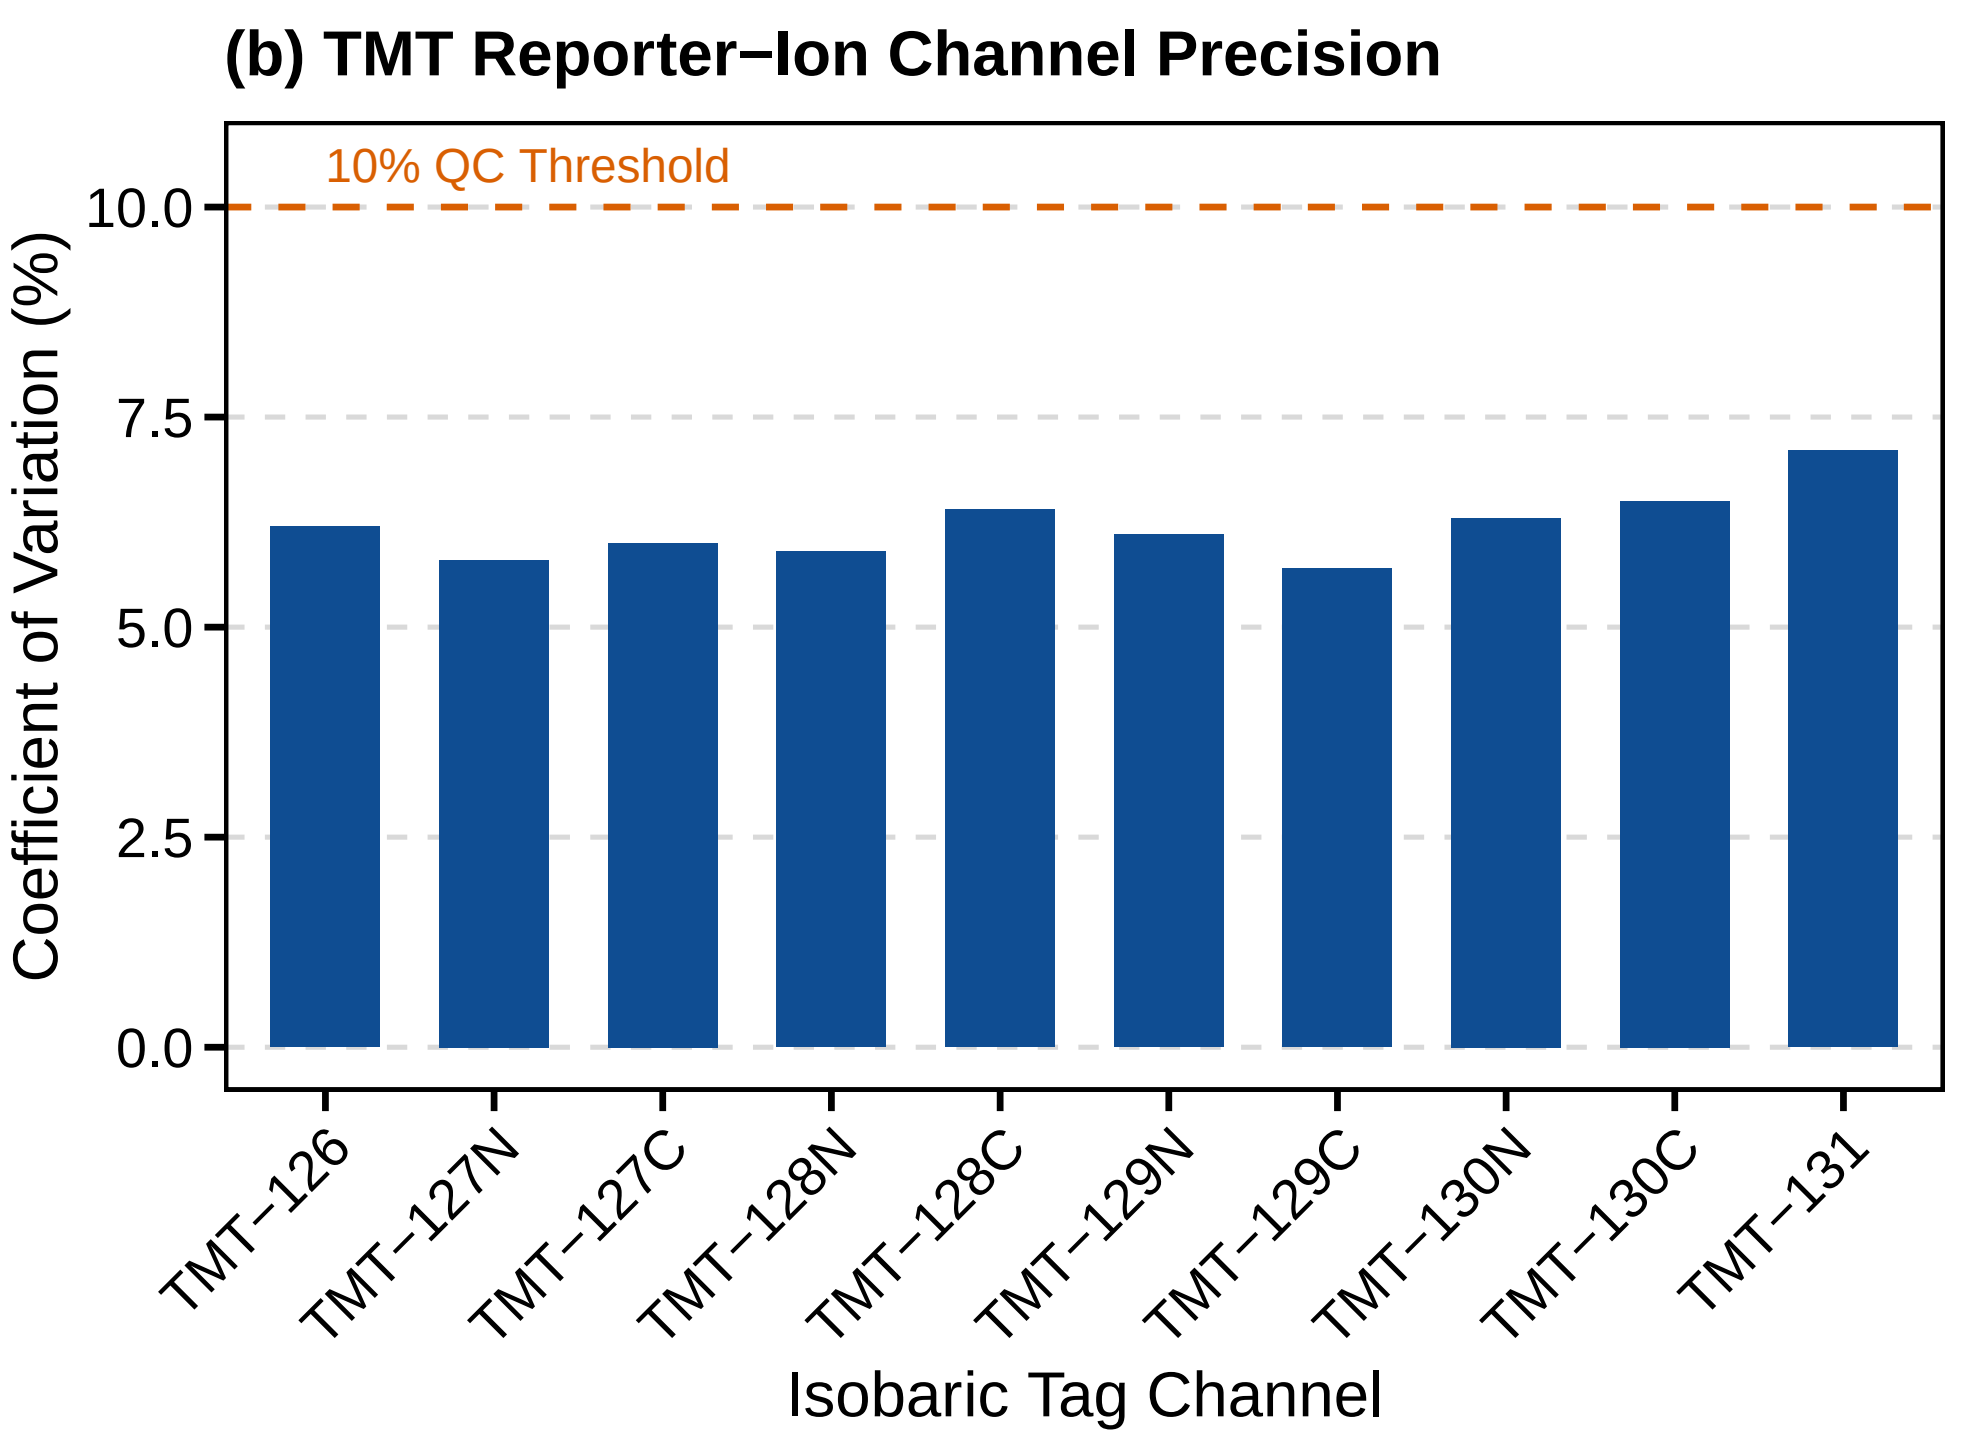
(b) TMT Reporter−Ion Channel Precision
10% QC Threshold
10.0
7.5
5.0
2.5
0.0
Coefficient of Variation (%)
TMT−126
TMT−127N
TMT−127C
TMT−128N
TMT−128C
TMT−129N
TMT−129C
TMT−130N
TMT−130C
TMT−131
Isobaric Tag Channel