Chromatogram Gallery of 9 Pure Metabolite Standards (MTBLS38)
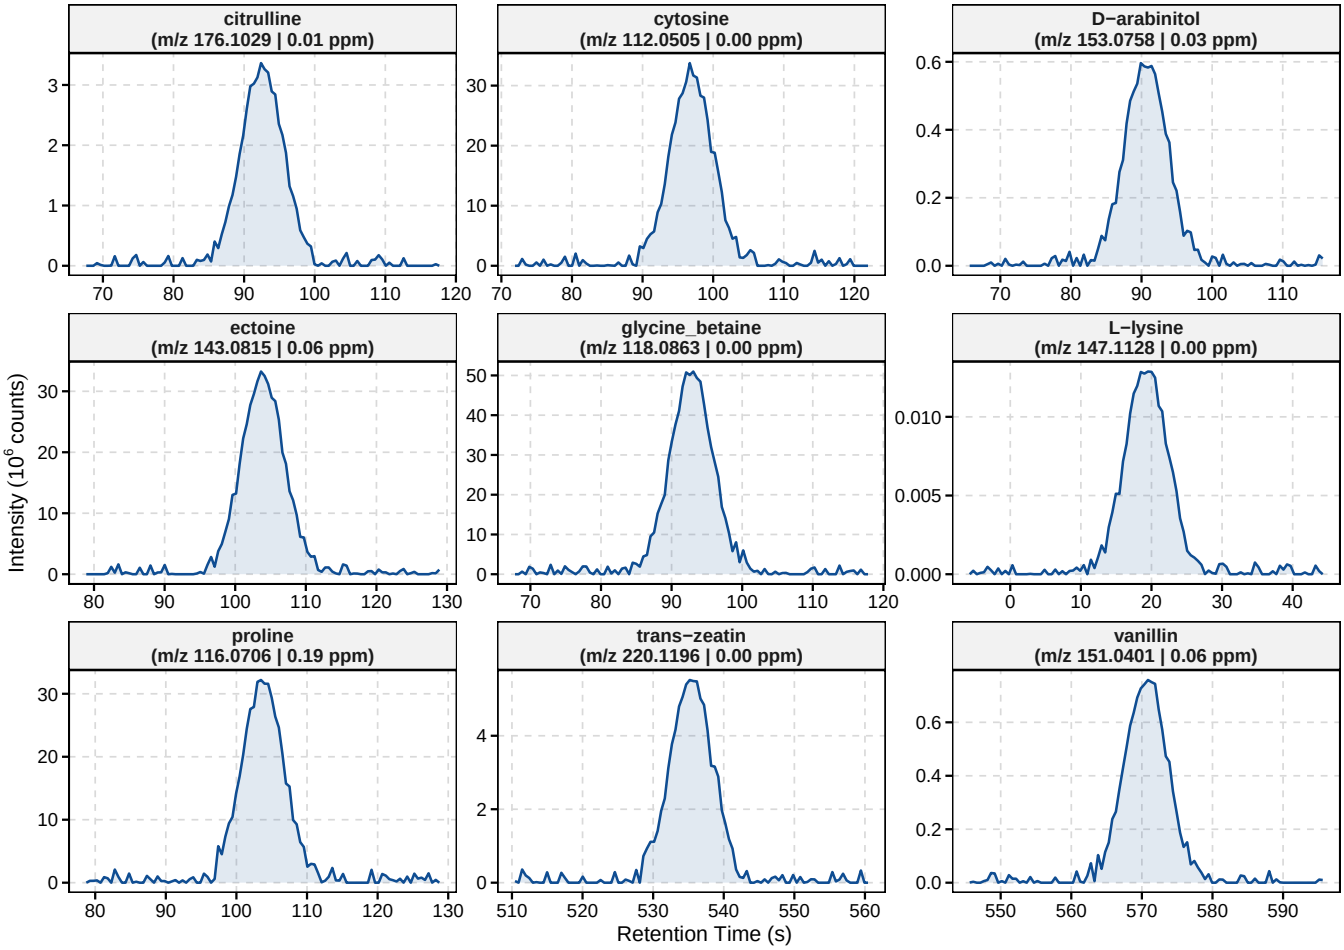
CentWave extracted ion chromatograms (±25 ppm window). All sub−ppm accuracy.