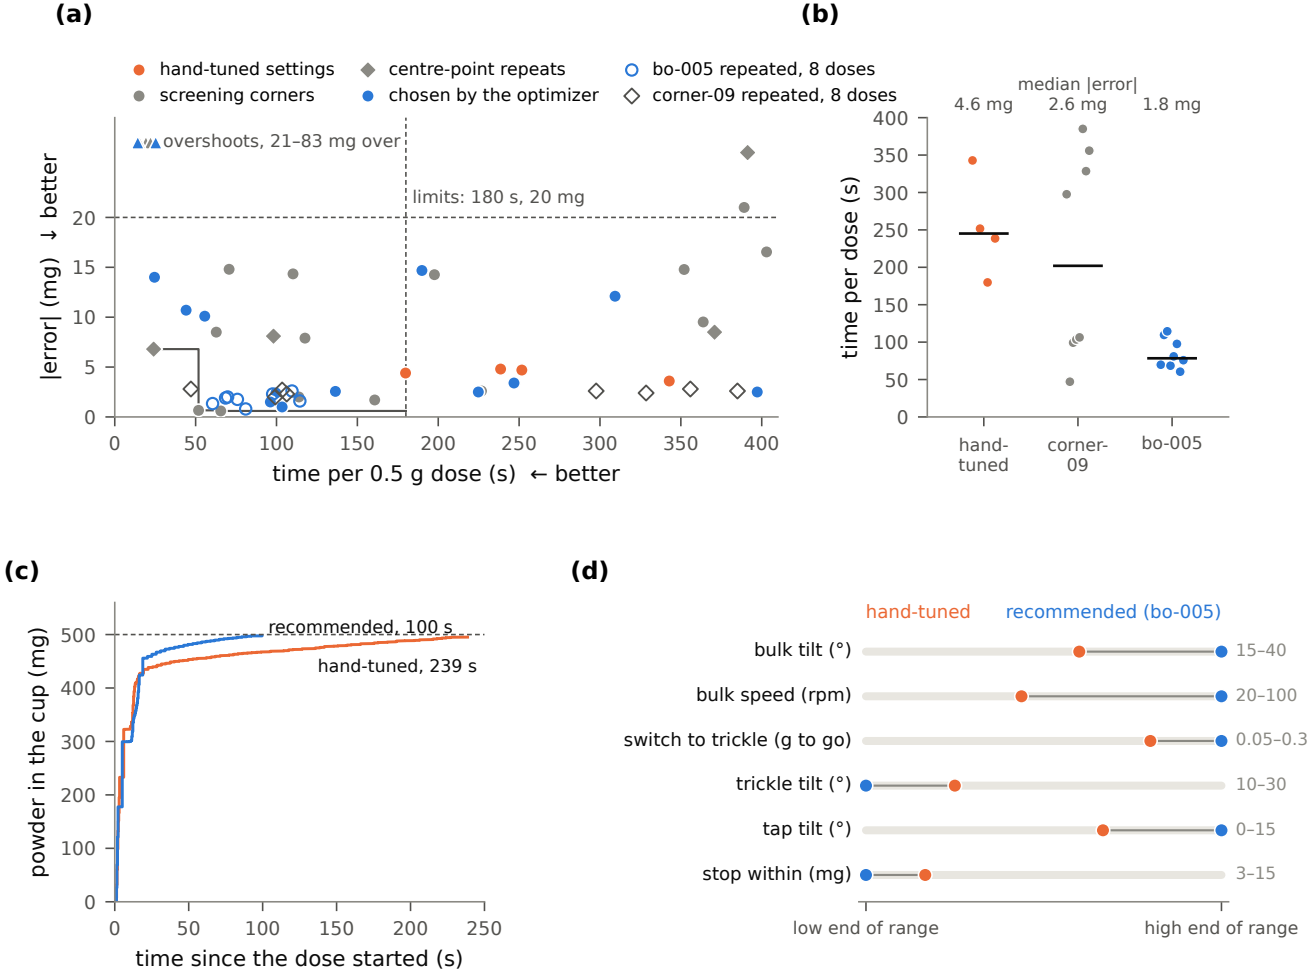
(a)
hand-tuned settings
screening corners
centre-point repeats
chosen by the optimizer
bo-005 repeated, 8 doses
corner-09 repeated, 8 doses
overshoots, 21–83 mg over
limits: 180 s, 20 mg
|error| (mg) ↓ better
time per 0.5 g dose (s) ← better
(b)
median |error|
4.6 mg
2.6 mg
1.8 mg
time per dose (s)
hand-tuned
corner-09
bo-005
(c)
recommended, 100 s
hand-tuned, 239 s
powder in the cup (mg)
time since the dose started (s)
(d)
hand-tuned
recommended (bo-005)
bulk tilt (°)
15–40
bulk speed (rpm)
20–100
switch to trickle (g to go)
0.05–0.3
trickle tilt (°)
10–30
tap tilt (°)
0–15
stop within (mg)
3–15
low end of range
high end of range