


Important Note:

The original schematic indicates the transformer uses a secondary = 100Vac; however the measurement seems to be a 50Vac.

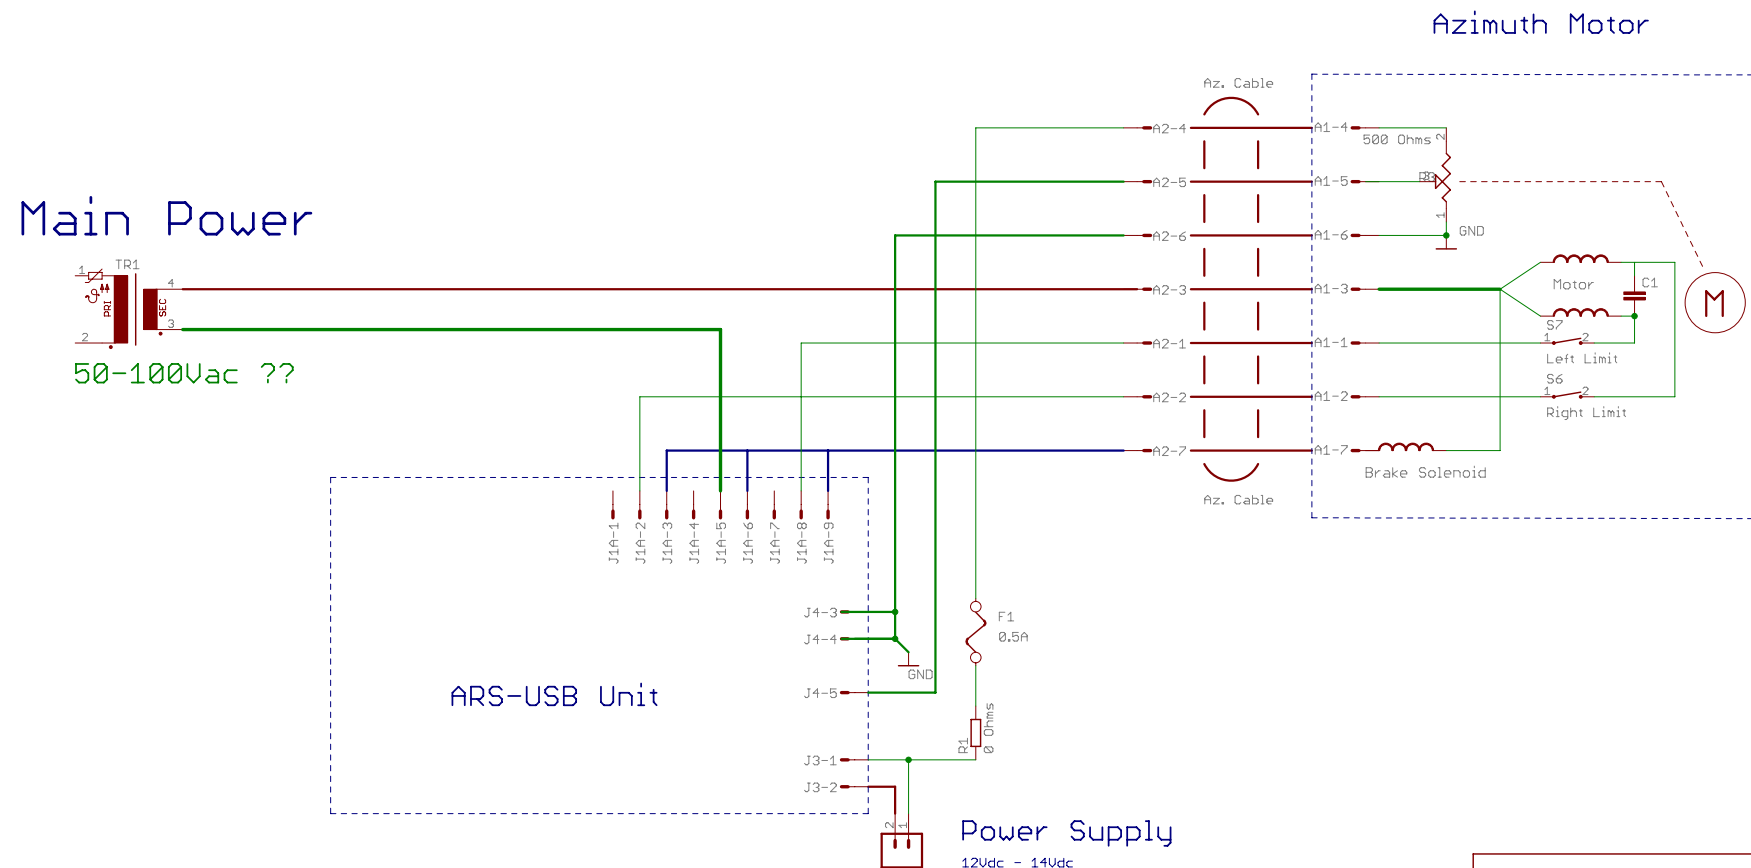

Emotator 1102/1103 control unit replacement	
TITLE: Emotator_1103	
Document Number:	REV:
Date: not saved!	Sheet: 1/1