

Model vs cardiologist labels — record 200

Threshold: 0.0434
Beats scored: 2580

Confusion matrix:

TP (model+annot agree abnormal):	778
TN (both agree normal):	1667
FP (model says abn, annot N):	67
FN (annot abn, model says N):	68

Sensitivity (recall): 0.920
Specificity: 0.961
Precision: 0.921
F1 score: 0.920


Per-beat-type breakdown:

N Normal	1734	flagged	3.9%
V PVC (ventricular ectopic)	815	flagged	95.5%
A Atrial premature	30	flagged	0.0%
F Fusion (V+N)	1	flagged	0.0%


Legend on next pages:

Blue line: bandpass-filtered ECG
Green tick: annotated NORMAL beat (cardiologist)
Magenta tick: annotated ABNORMAL beat (cardiologist)
Red shading: beat the MODEL flagged as anomaly
An ideal model has red shading exactly under magenta ticks.


Record 200 — t=30-50 s

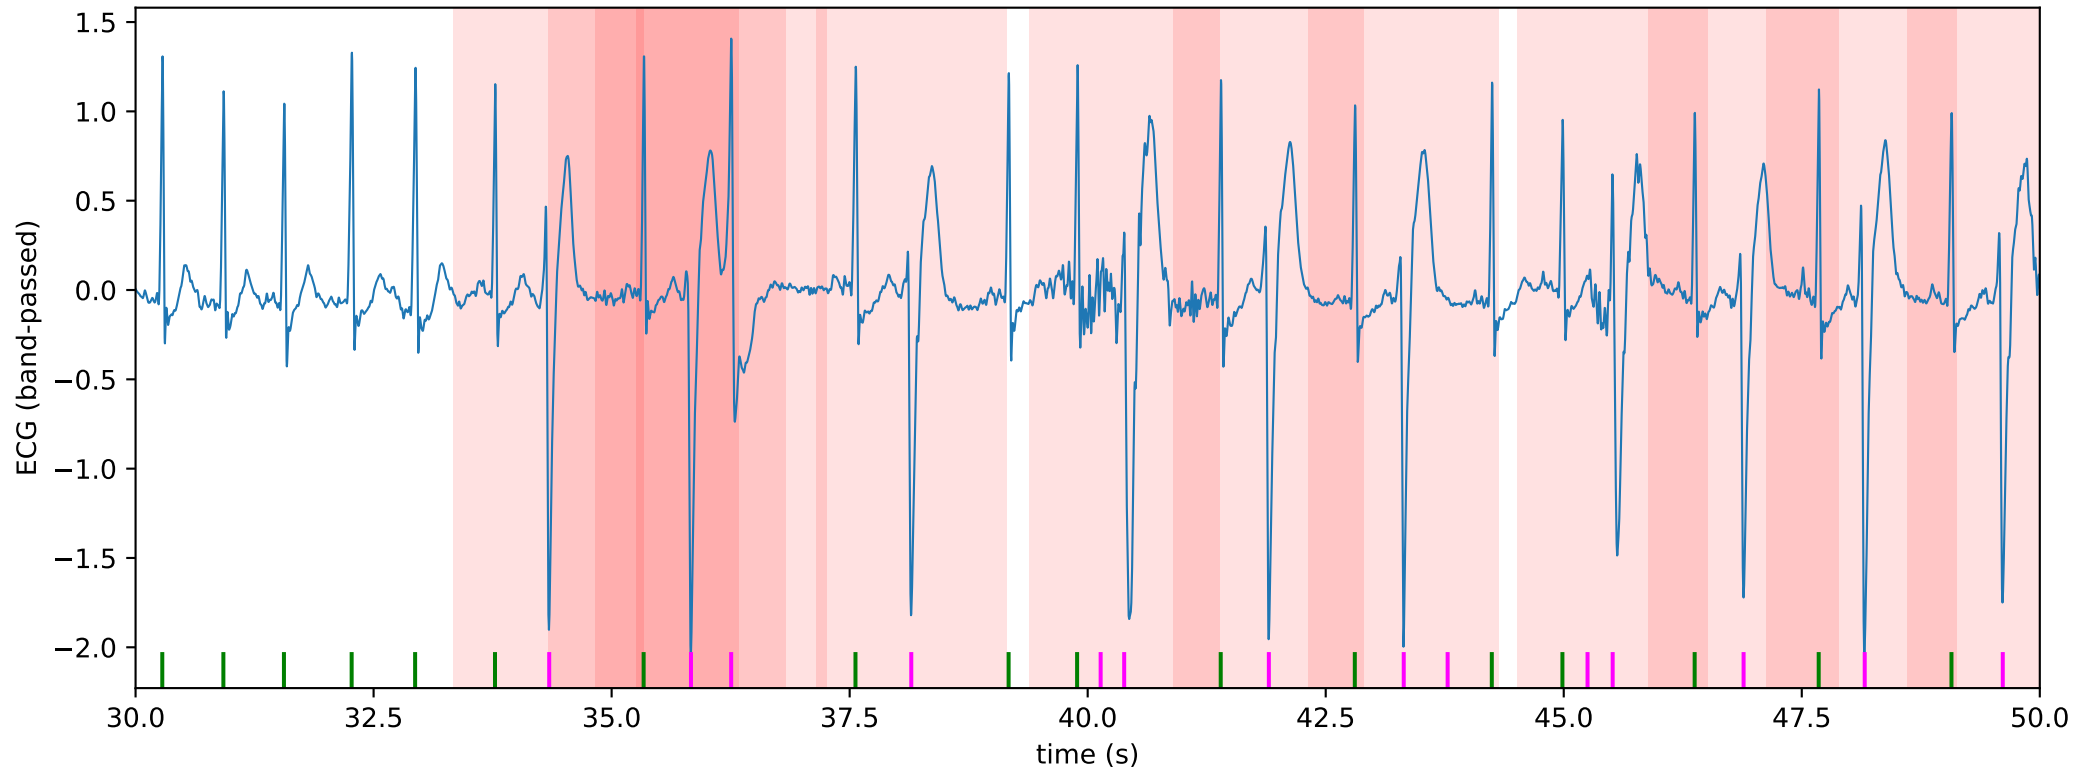


Record 200 — t=50-70 s

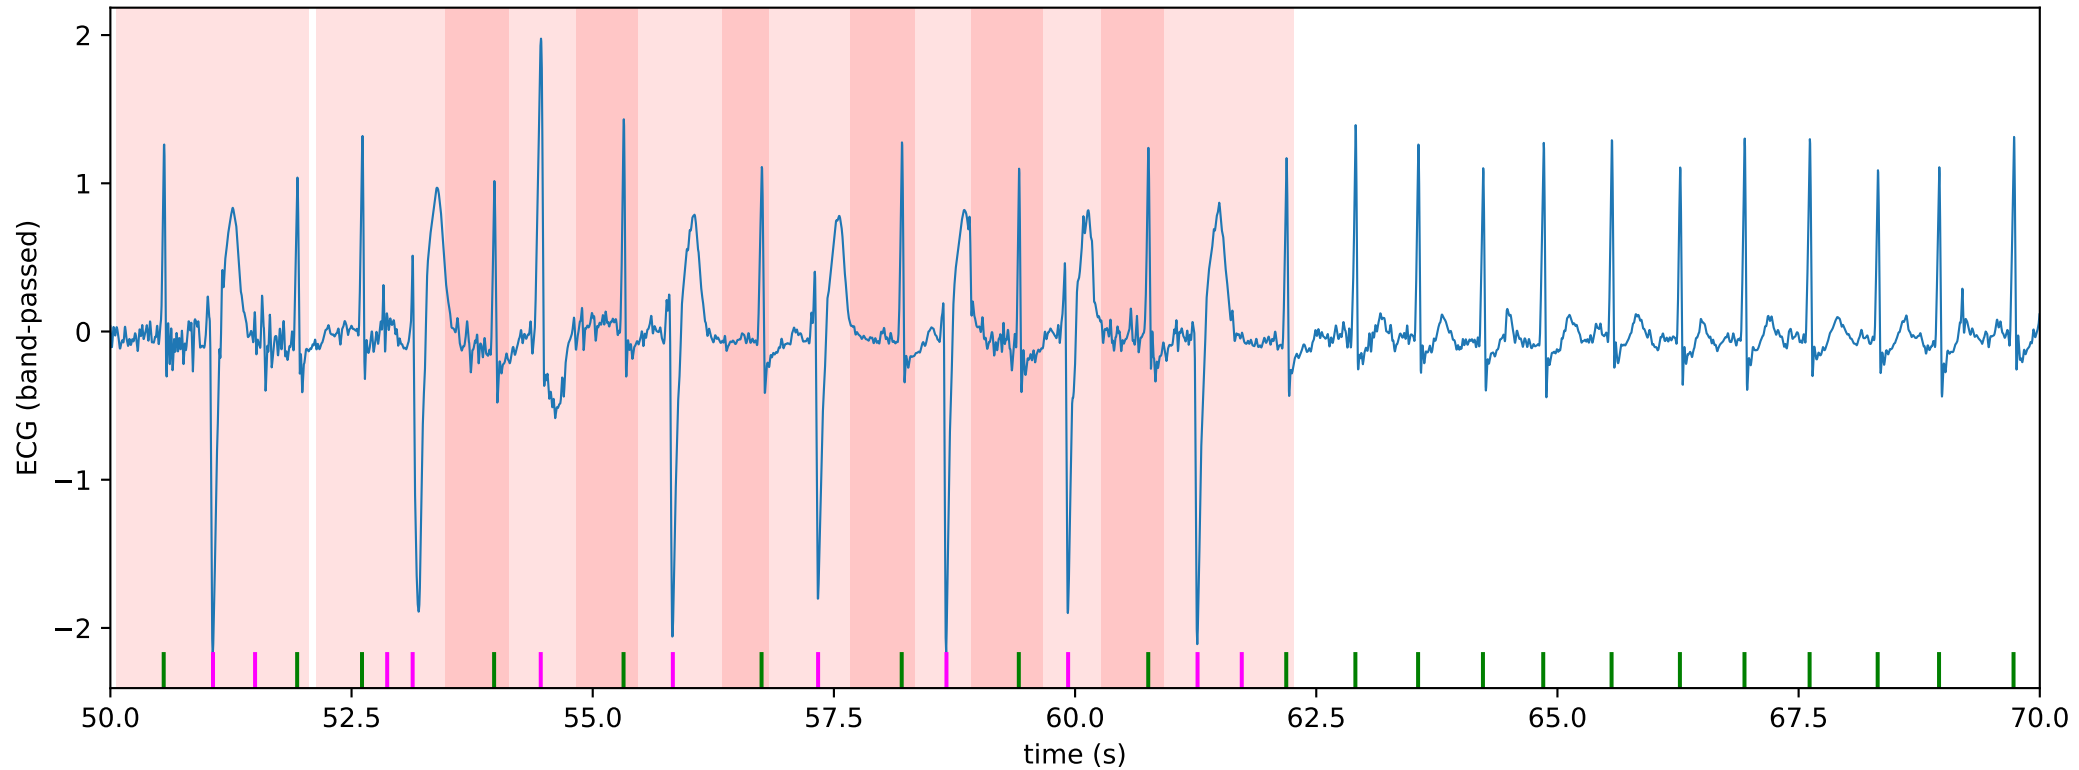


Record 200 — t=70-90 s

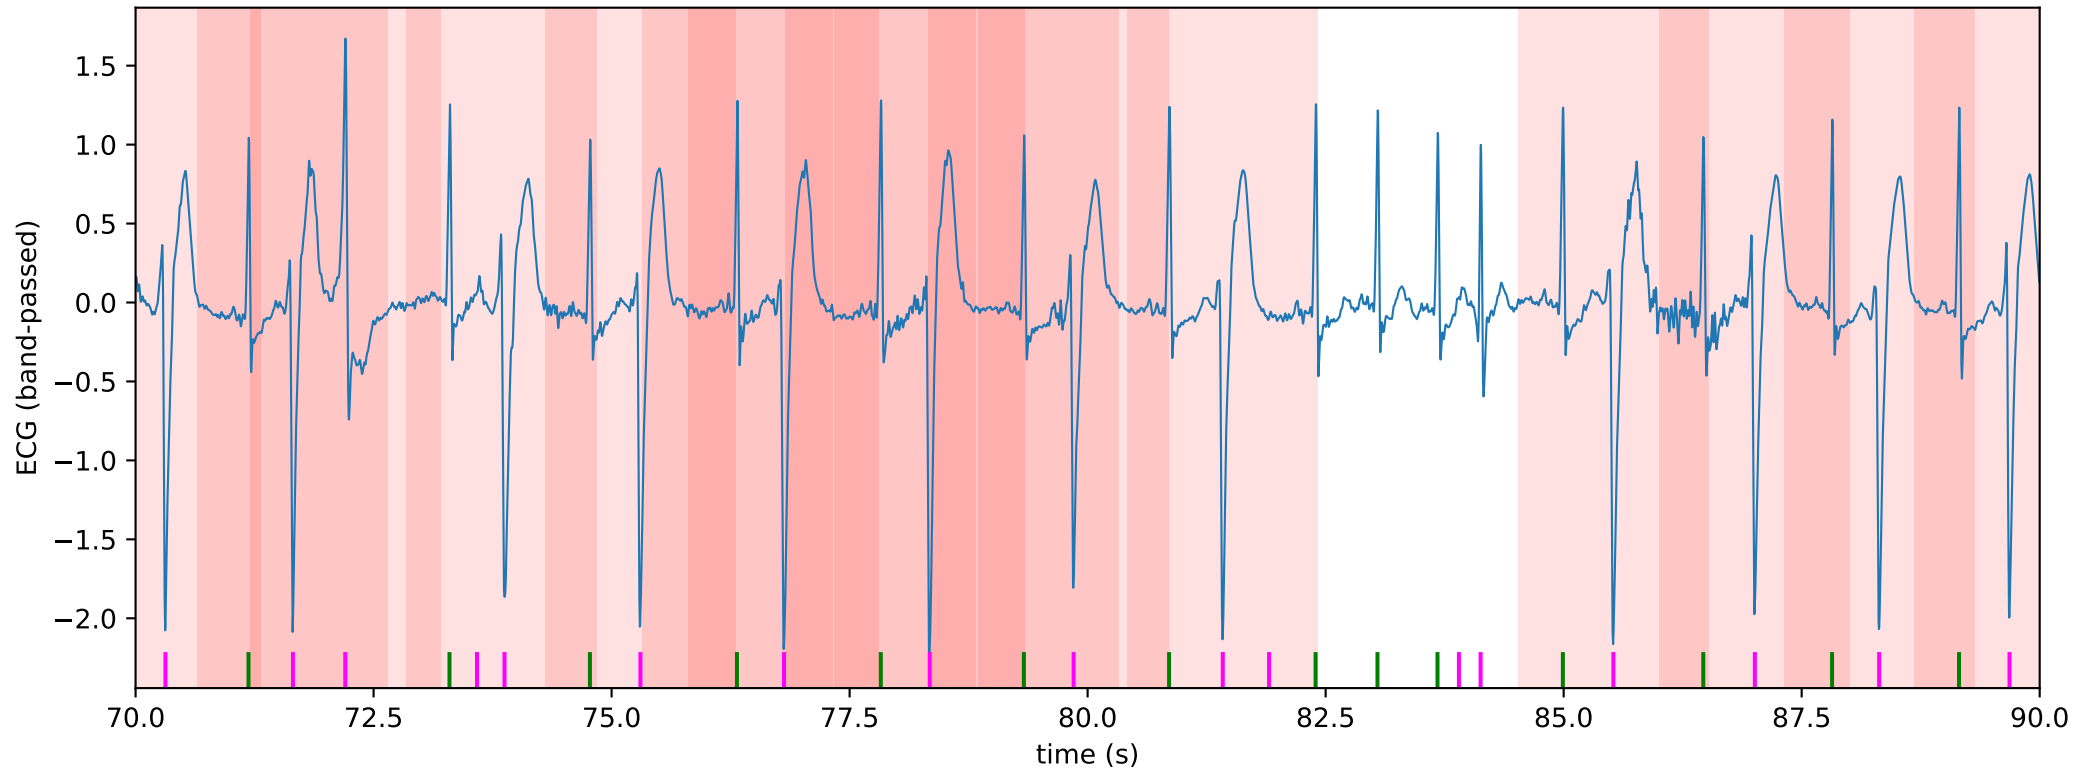

Record 200 — t=90-110 s

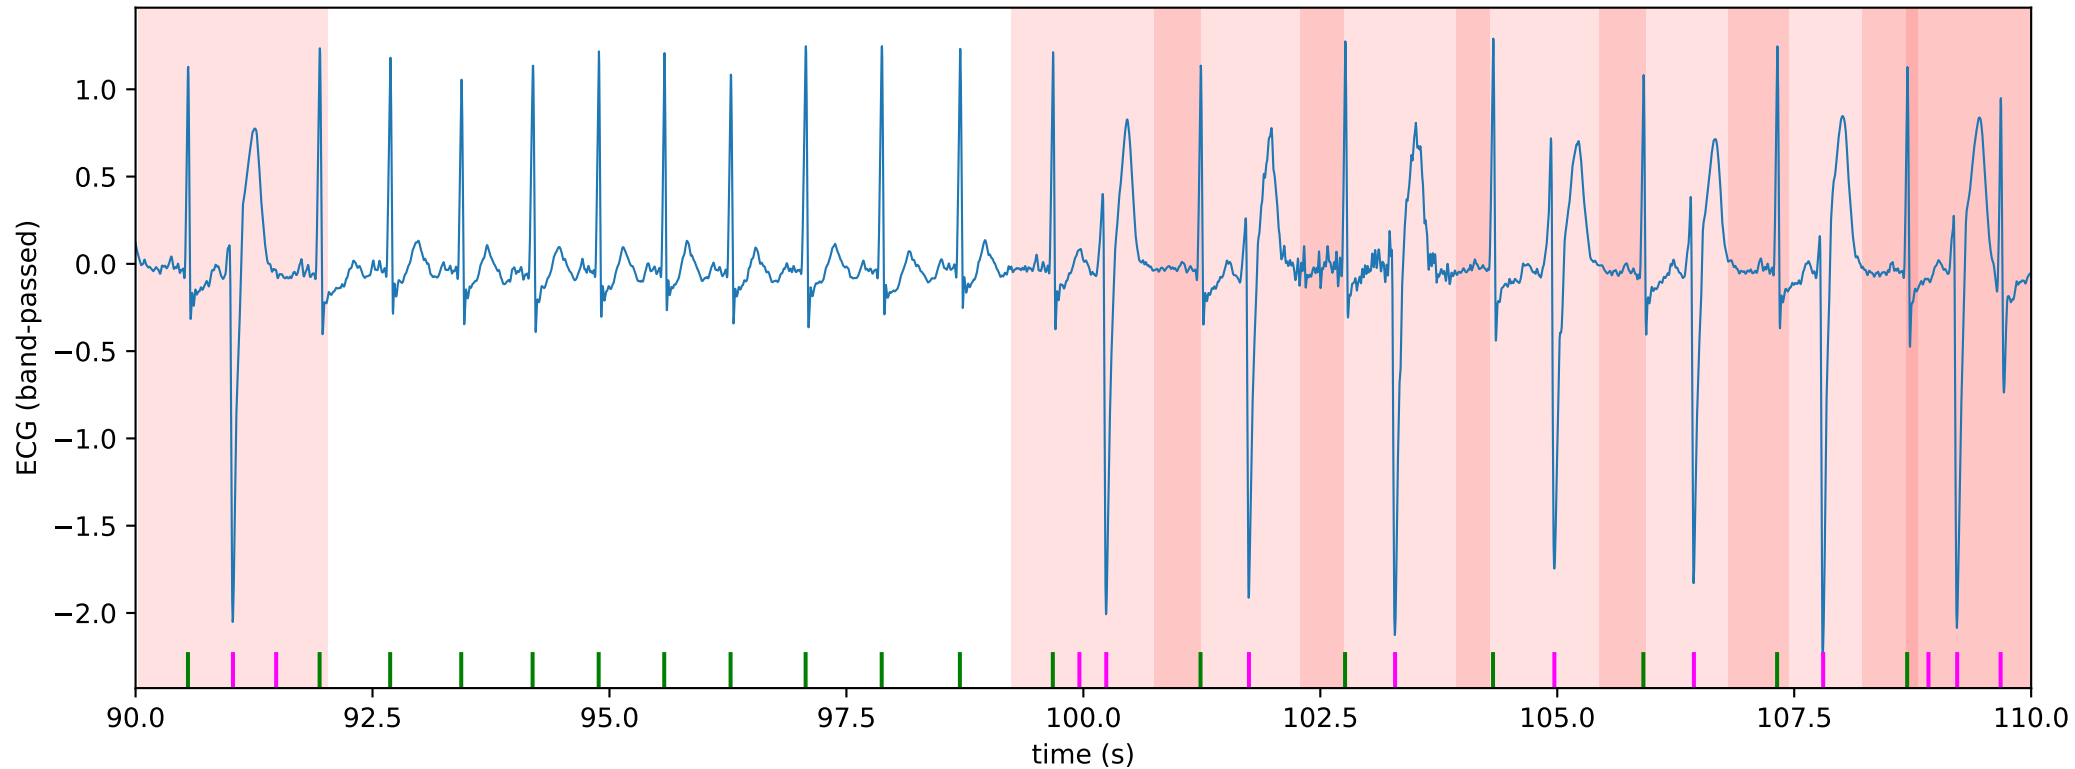

Record 200 — t=110-130 s

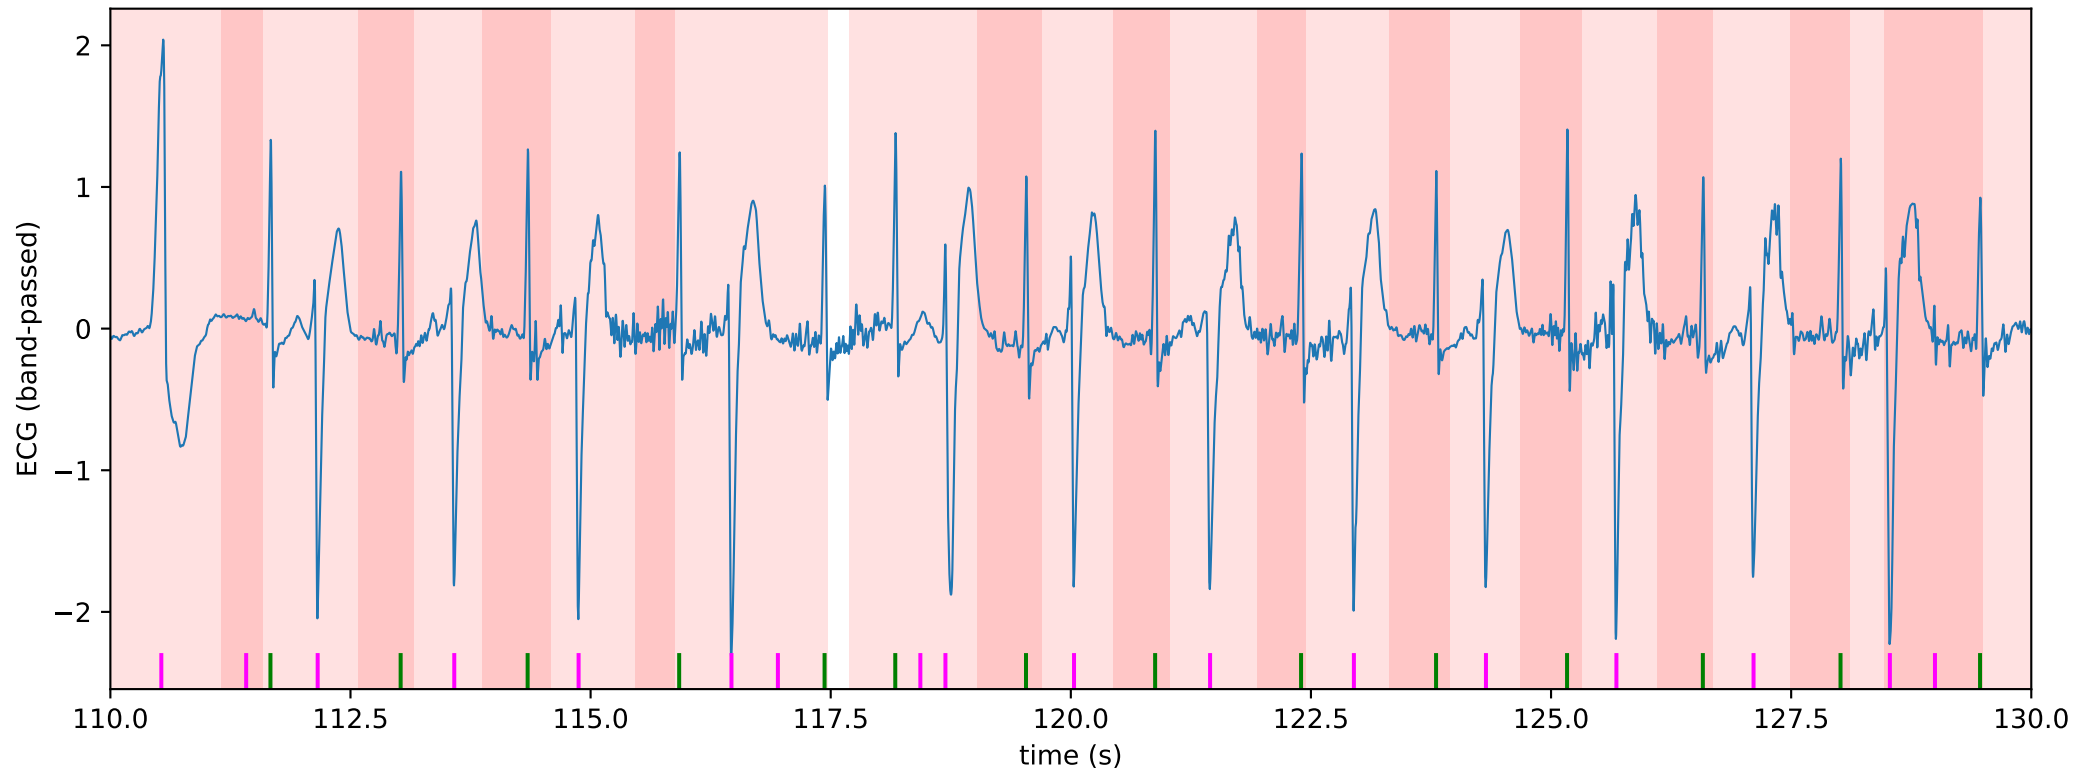

Record 200 — t=130-150 s

