

Model vs cardiologist labels — record 208

Threshold: 0.0434
Beats scored: 2711

Confusion matrix:

TP (model+annot agree abnormal): 867
TN (both agree normal): 1507
FP (model says abn, annot N): 58
FN (annot abn, model says N): 279

Sensitivity (recall): 0.757
Specificity: 0.963
Precision: 0.937
F1 score: 0.837


Per-beat-type breakdown:

N Normal	1560	flagged	3.4%
V PVC (ventricular ectopic)	777	flagged	98.5%
F Fusion (V+N)	366	flagged	27.6%
?	5	flagged	100.0%
S Supraventricular	2	flagged	0.0%
Q Unclassifiable	1	flagged	100.0%


Legend on next pages:

Blue line: bandpass-filtered ECG
Green tick: annotated NORMAL beat (cardiologist)
Magenta tick: annotated ABNORMAL beat (cardiologist)
Red shading: beat the MODEL flagged as anomaly
An ideal model has red shading exactly under magenta ticks.


Record 208 — t=30-50 s

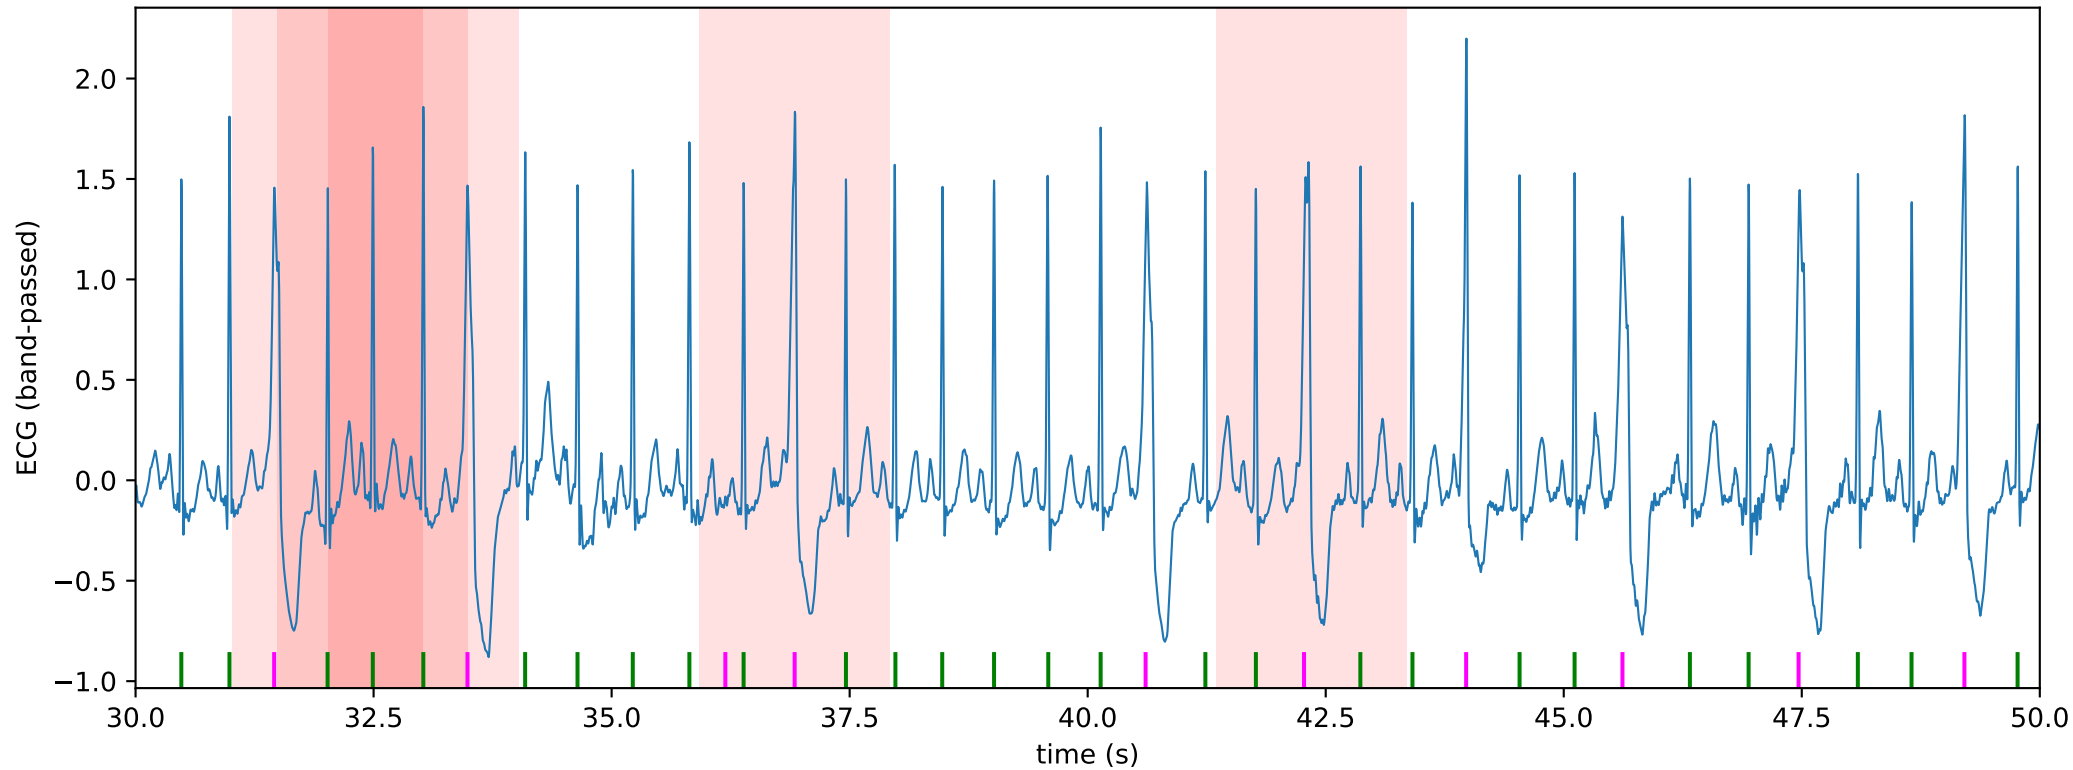


Record 208 — t=50-70 s

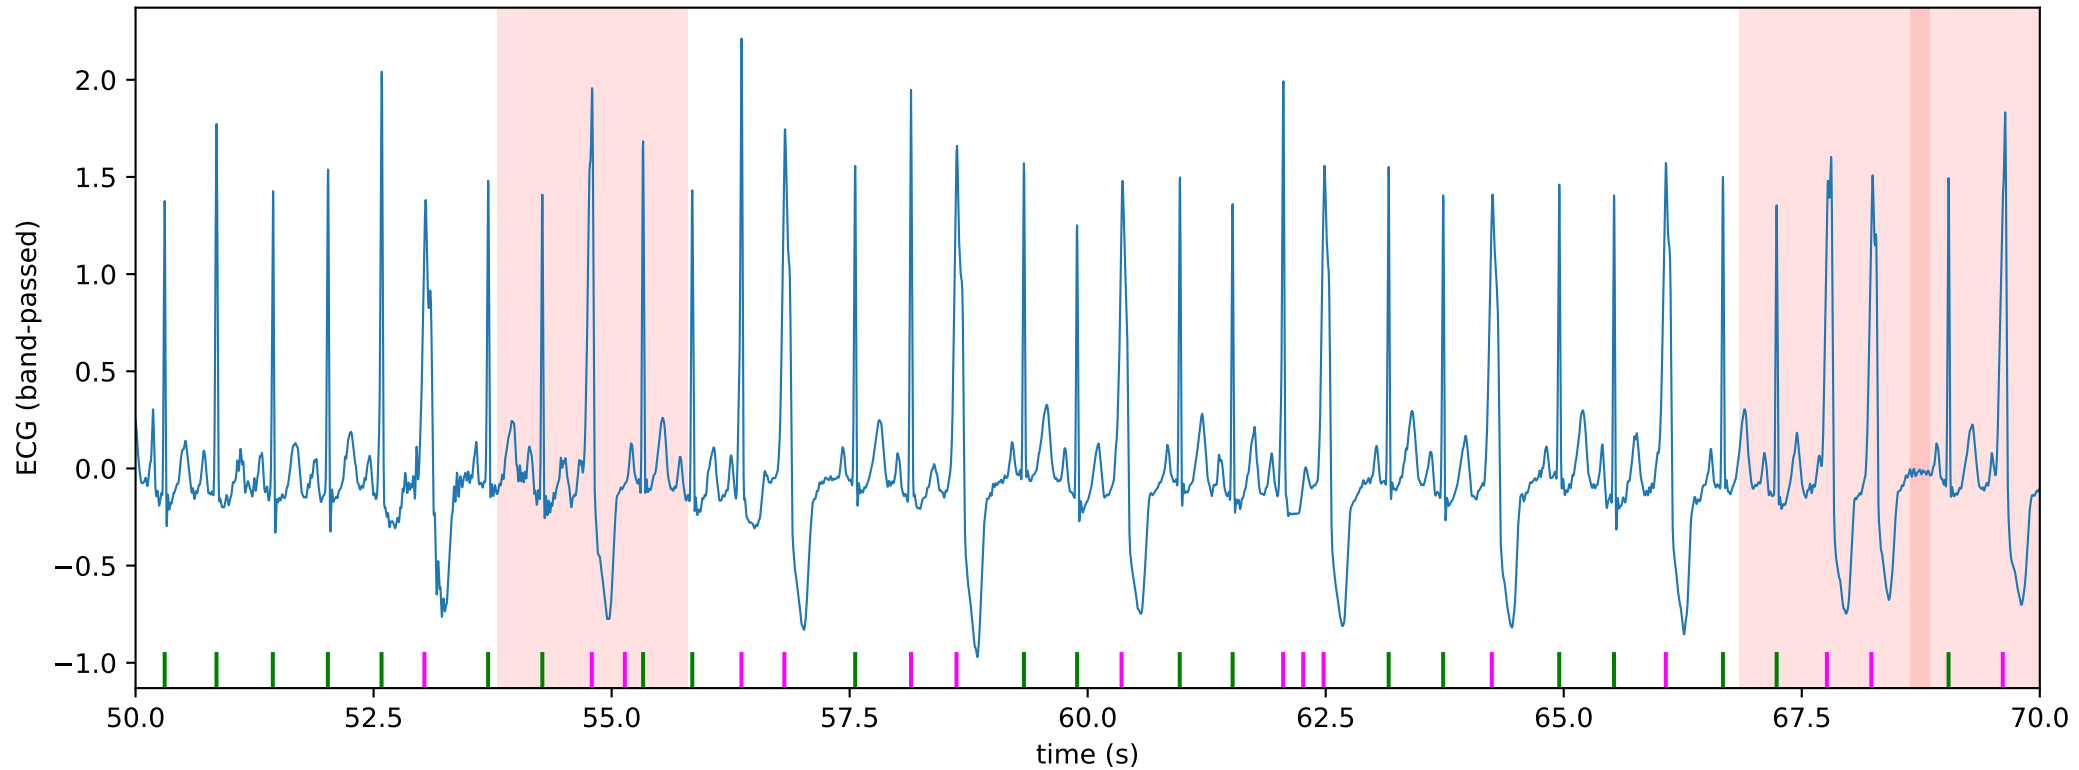


Record 208 — t=70-90 s

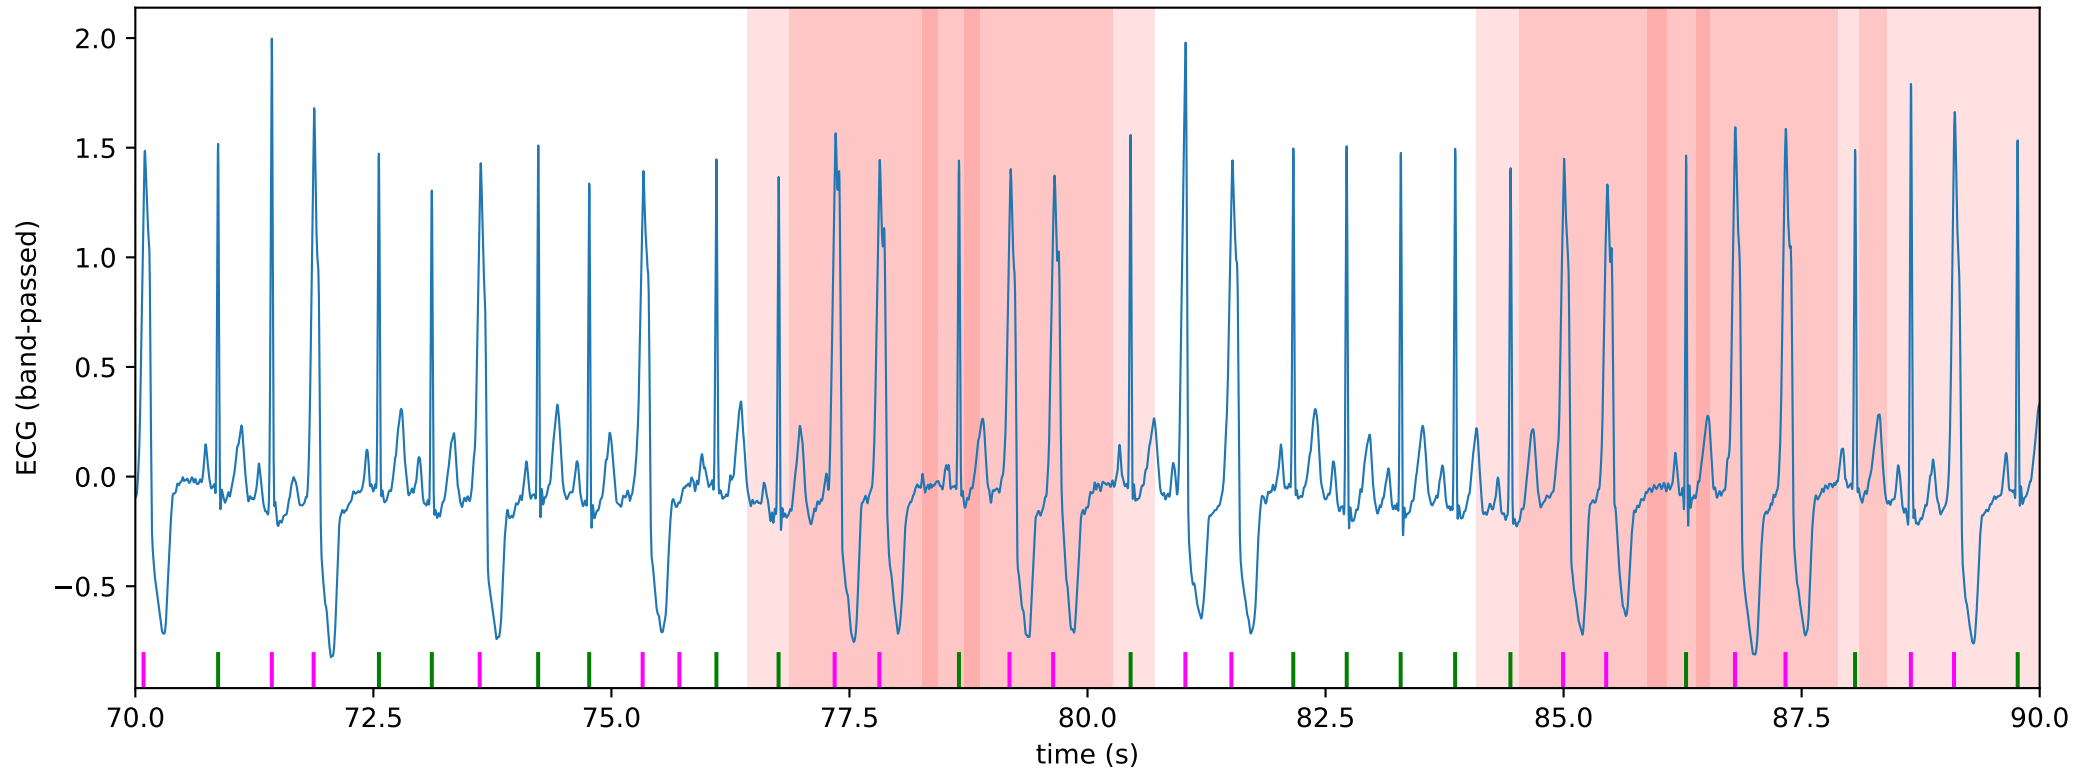

Record 208 — t=90-110 s

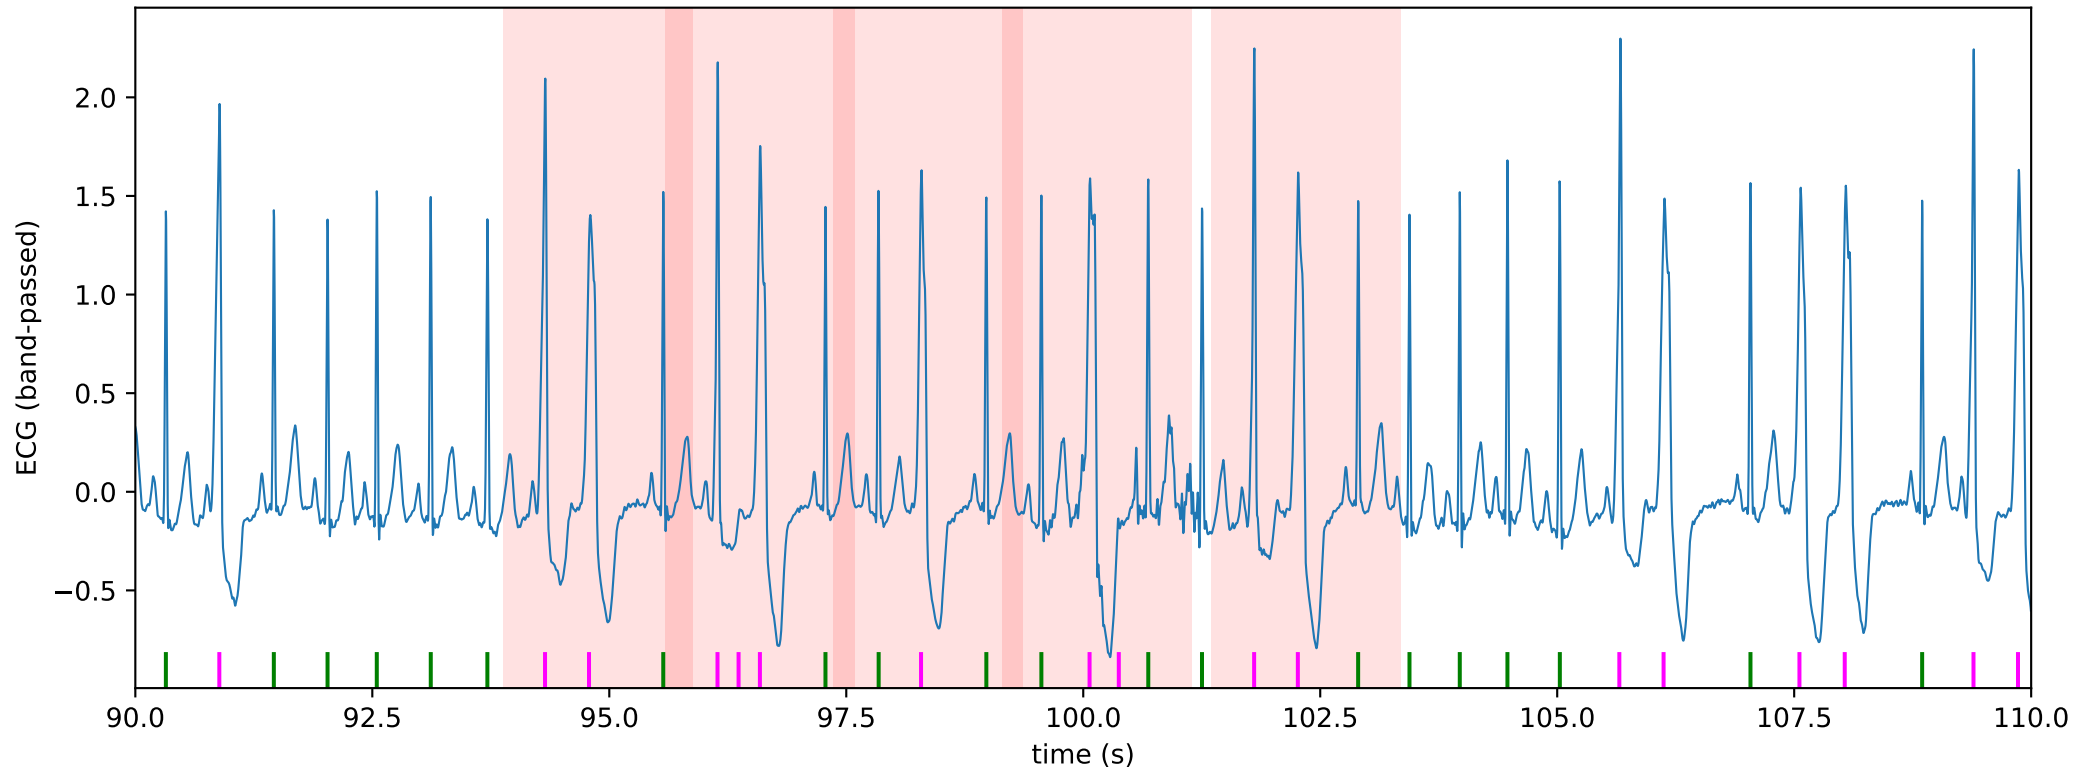

Record 208 — t=110-130 s

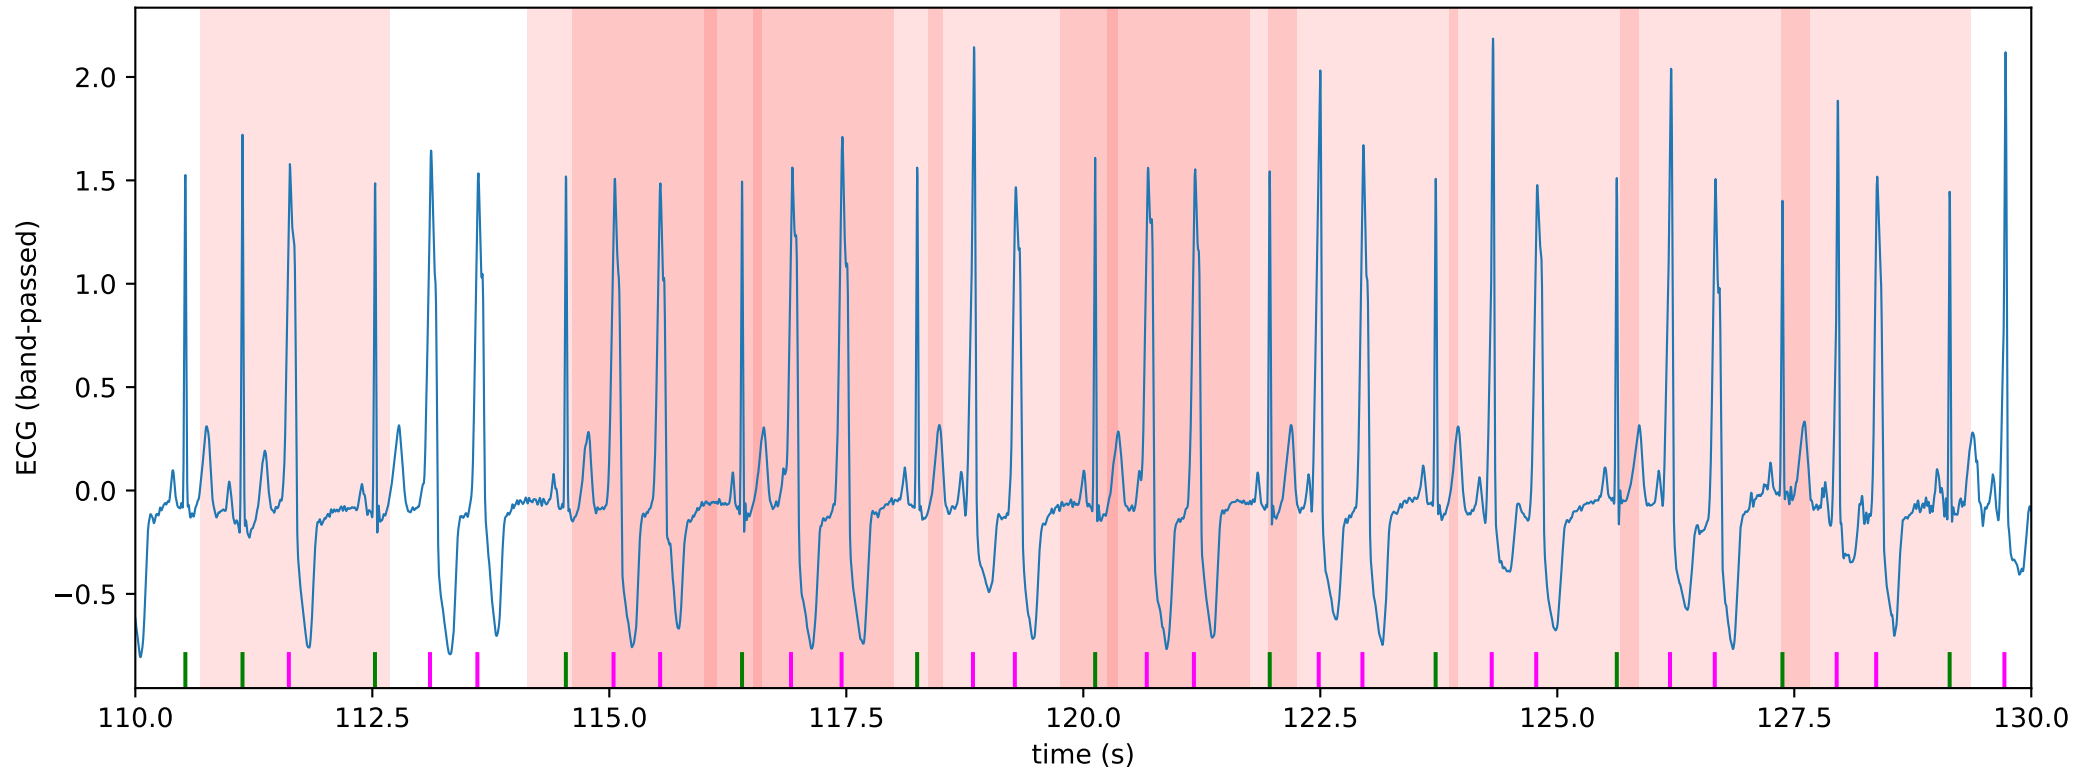

Record 208 — t=130-150 s

