


Title		
Tuned Collector Oscillator		
Size	Document Number	Rev
A	<Doc>	<RevCode>
Date: Friday, March 01, 2024		Sheet 1 of 1

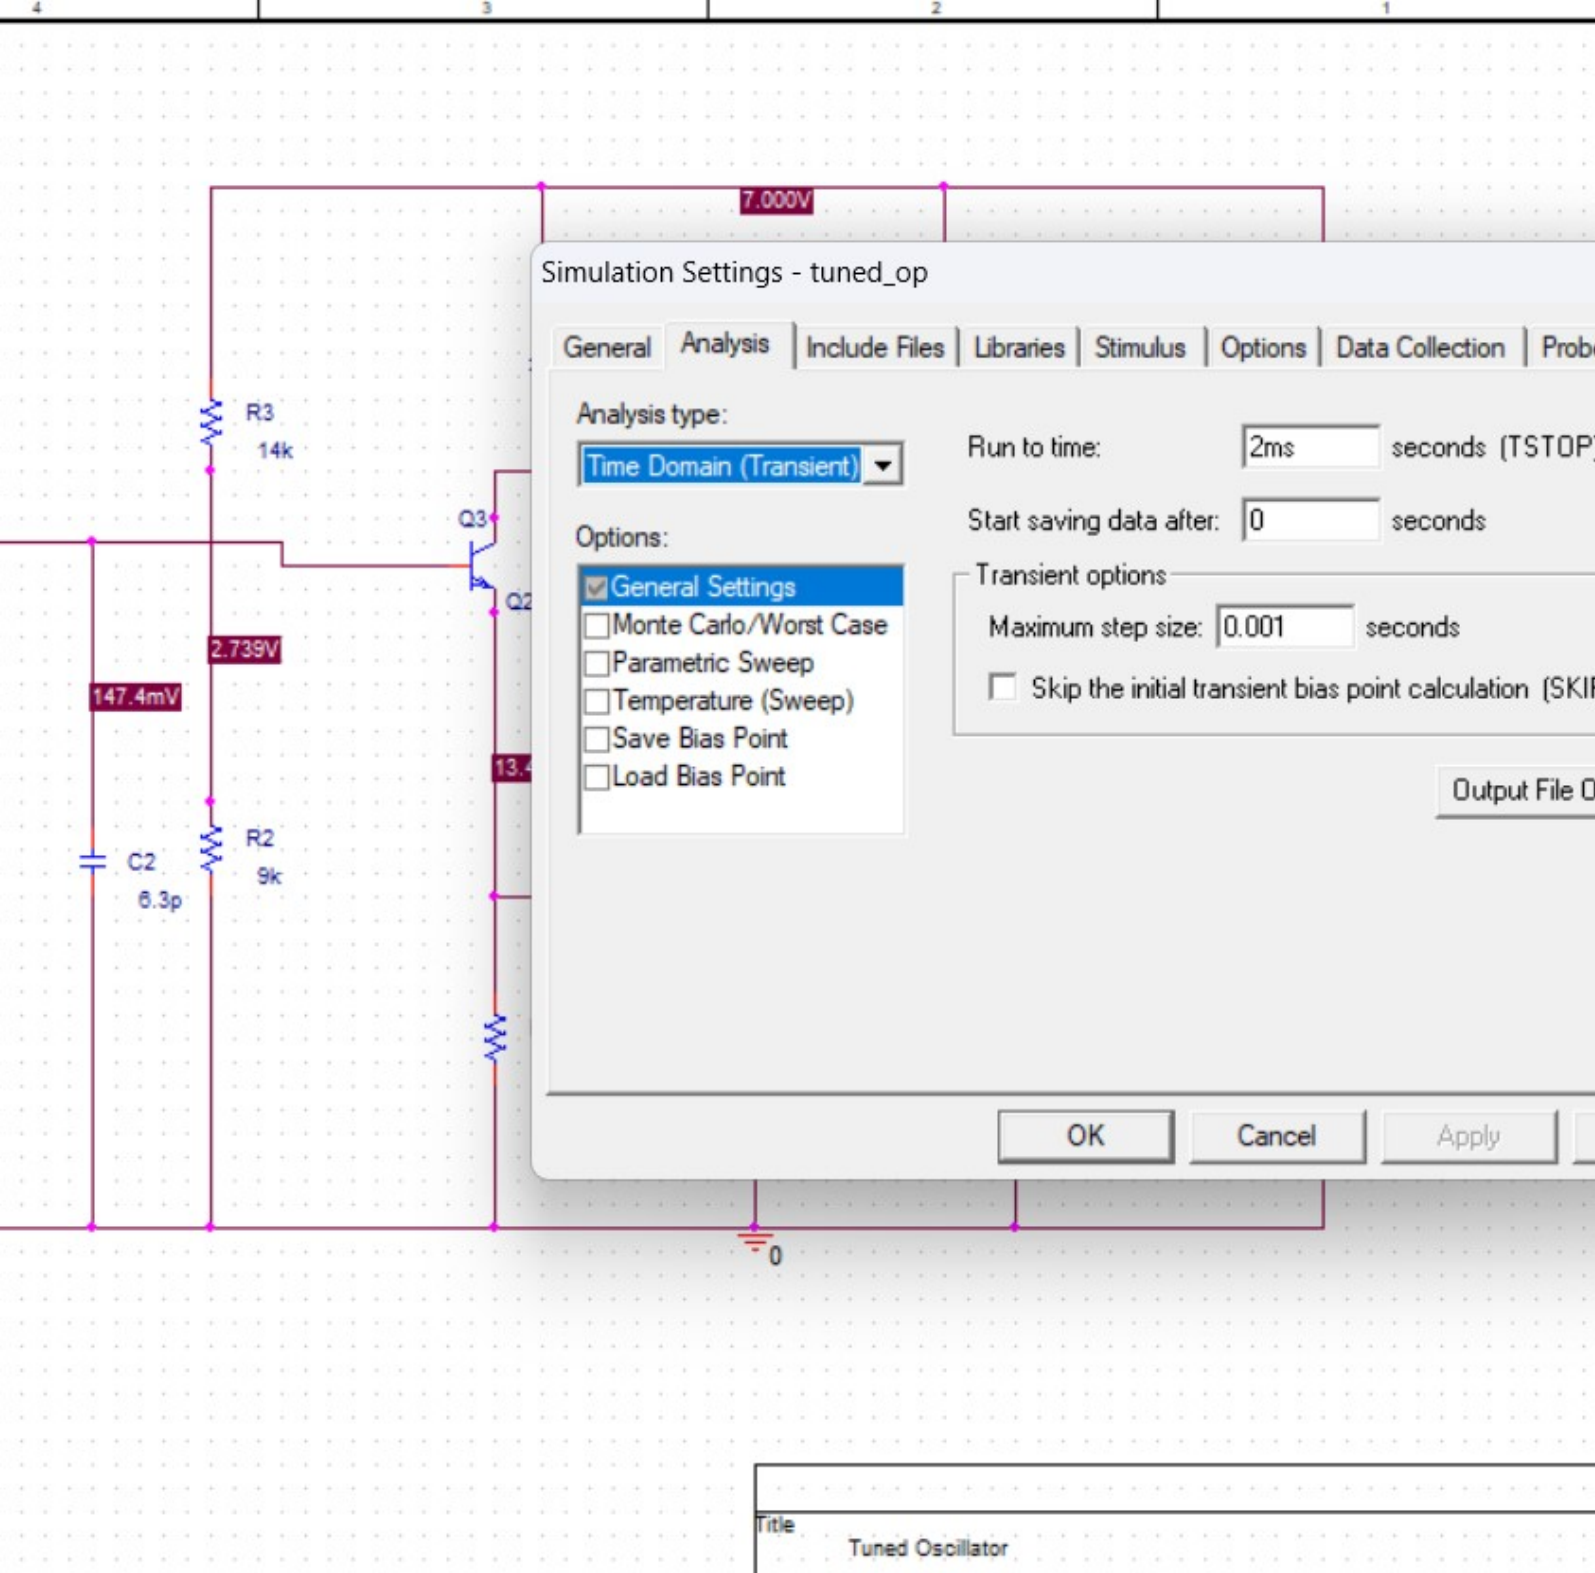

Simulation Settings - tuned_op

General Analysis Include Files Libraries Stimulus Options Data Collection Probe Window

Analysis type:
Time Domain (Transient)

Run to time: 2ms seconds (TSTOP)

Start saving data after: 0 seconds

Options:

- ☒ General Settings
- ☐ Monte Carlo/Worst Case
- ☐ Parametric Sweep
- ☐ Temperature (Sweep)
- ☐ Save Bias Point
- ☐ Load Bias Point

Transient options

Maximum step size: 0.001 seconds

☐ Skip the initial transient bias point calculation (SKIPBP)

Output File Options...

OK Cancel Apply Help

Title
Tuned Oscillator

