HEMOSCAN AI


BLOOD SMEAR IMAGE ANALYSIS REPORT

AI-assisted research report • Not a diagnostic laboratory result

1. SPECIMEN AND REPORT DETAILS

Sample ID	SAMPLE-A875C723
Analysis ID	a875c7231f1946fcbaad8bbaf1c70d01
Report generated	25 Oct 2026, 04:13:58 India Standard Time
AI model file	best.pt
Review status	Pending human review

2. ANNOTATED BLOOD SMEAR IMAGE

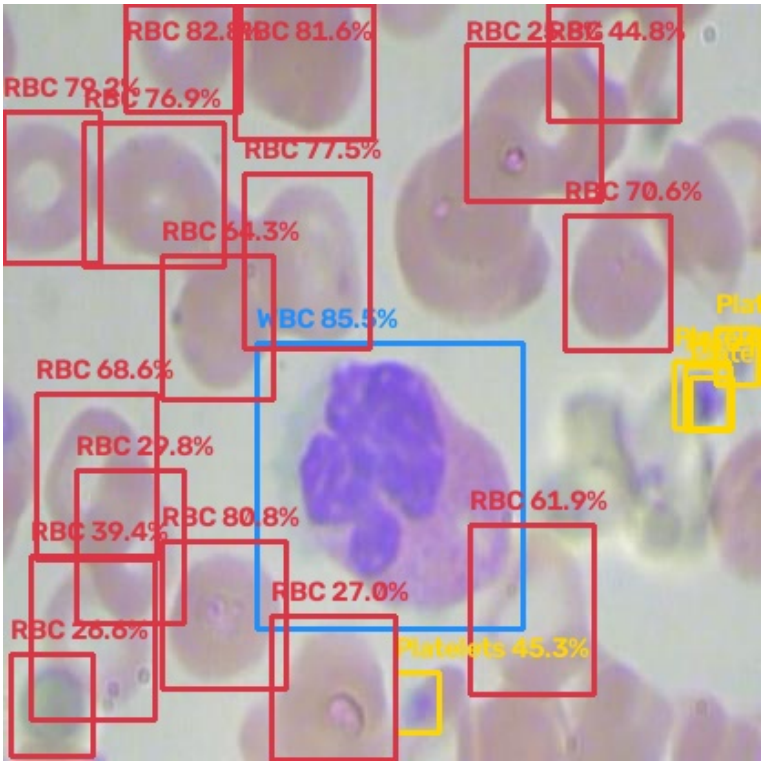

Detections and labels shown are model-generated and require review.

3. DETECTION SUMMARY

Cell class	Detected objects	Share of detections
RBC	16	72.7%
WBC	1	4.5%
Platelets	5	22.7%
TOTAL	**22**	**100.0%**

4. MODEL CONFIDENCE

Mean model confidence: 57.0%

Confidence is the model's score for its detections; it is not a measure of diagnostic accuracy.

5. IMAGE QUALITY REVIEW

Image dimensions: 416 × 416 pixels

Blur indicator (Laplacian variance): 8.77

Mean brightness: 179.39

Contrast indicator: 19.89


Quality status: Review recommended

Quality warnings:

• Possible blur detected. Consider capturing a sharper image.

• Low image contrast may affect detection quality.

6. CELL DISTRIBUTION CHART

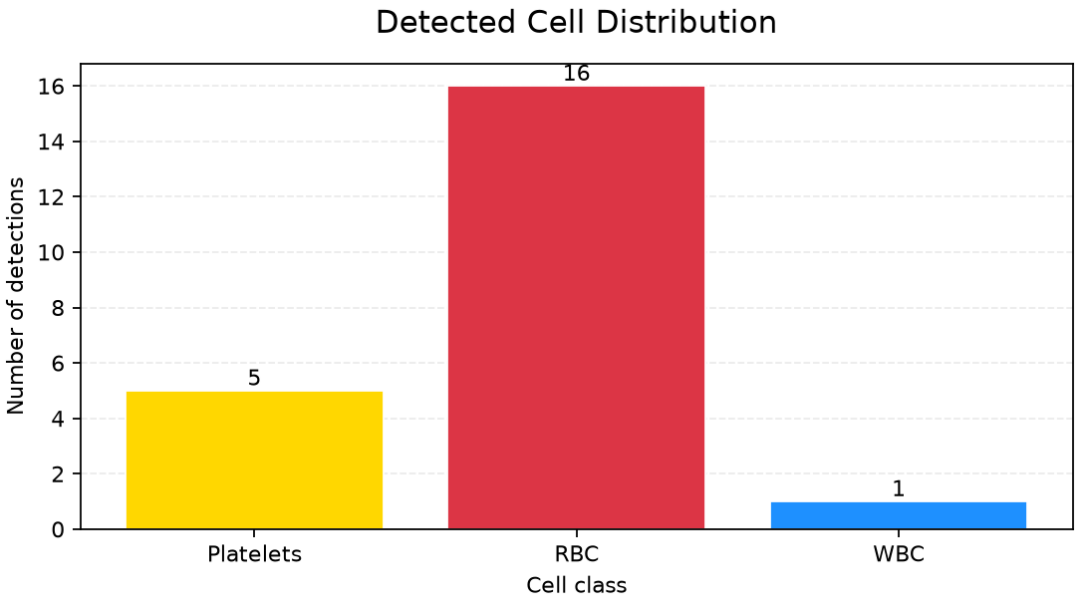

7. AUTOMATED DETECTION CONCLUSION

Interpretation status	Requires professional review
Finding	The AI model detected 22 objects: 16 red blood cell (RBC) detections, 1 white blood cell (WBC) detections, and 5 platelet detections.
Finding	The image-quality checks raised 2 warning(s). These may affect detection reliability.
Finding	The mean model confidence across detected objects was 57.0%. Confidence is not a measure of diagnostic accuracy.
Recommendation	Review the image-quality warnings and consider recapturing the image before interpreting the results.
Recommendation	Have the annotated image and detections reviewed by a qualified laboratory professional.
Recommendation	Do not use these image-level counts alone to diagnose a disease or determine whether a blood count is normal or abnormal.

8. LABORATORY REVIEW

Reviewer name	_____
Signature	_____
Review date	_____
Comments	_____ _____

IMPORTANT MEDICAL DISCLAIMER

This report was generated by an AI-based research and educational prototype. Counts represent model detections in the uploaded image, not validated blood-cell concentrations or a complete blood count. Image-quality checks are heuristic. These results must not be used alone for diagnosis, treatment, or clinical decision-making. Review by a qualified laboratory professional and appropriate validation are required before any clinical use.