



## Calibration Report

Instrument Used : Agilent DSA-X 93204A 33GHz - 80GSa/s Digital Signal Analyzer

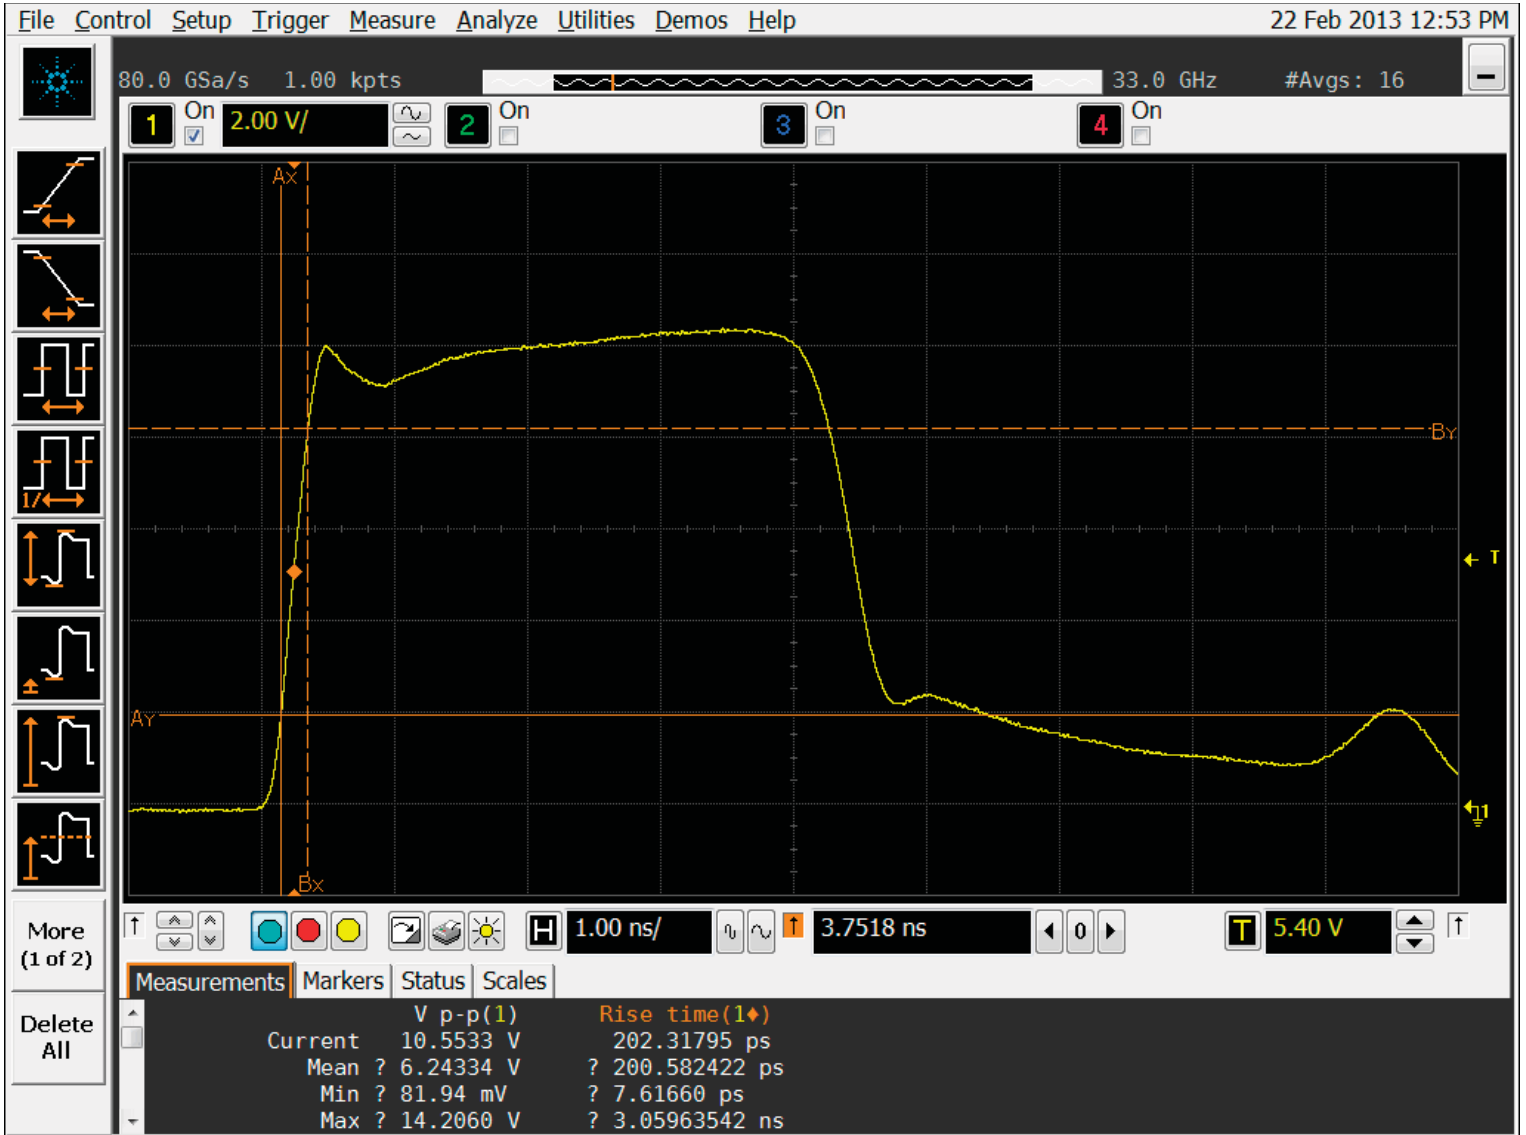

Rise time is measured between 20%to 80% of the signal Vpp into a 50 ohm measurement plane at the pulse generators connector

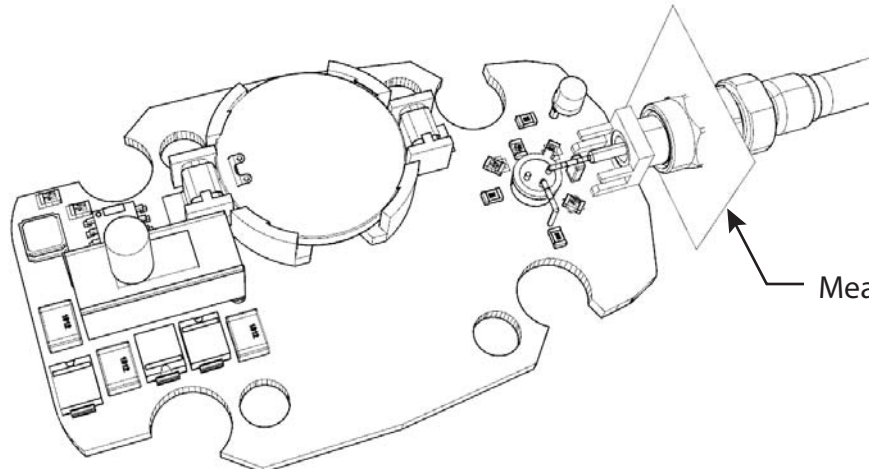

Measurement plane