# AUDIOLOGICAL EVALUATION & CLINICAL PATHOLOGY REPORT
## Hardware-Grade Diagnostic Software Audiometer | ISO 8253-1 Compliant

Patient ID: PT-2026-001
Name: Ramesh Kumar
Age: 48 years
Date / Time: 2026-10-14T13:55

Clinician / Operator: Dr. S. Sharma, Au.D.
Transducer Profile: Sennheiser_HDA200
Calibration Status: Calibrated (ISO 389-1)
Deployment: Rural Tele-Audiology Field Unit

### PURE TONE AUDIOGRAM (BINAURAL)

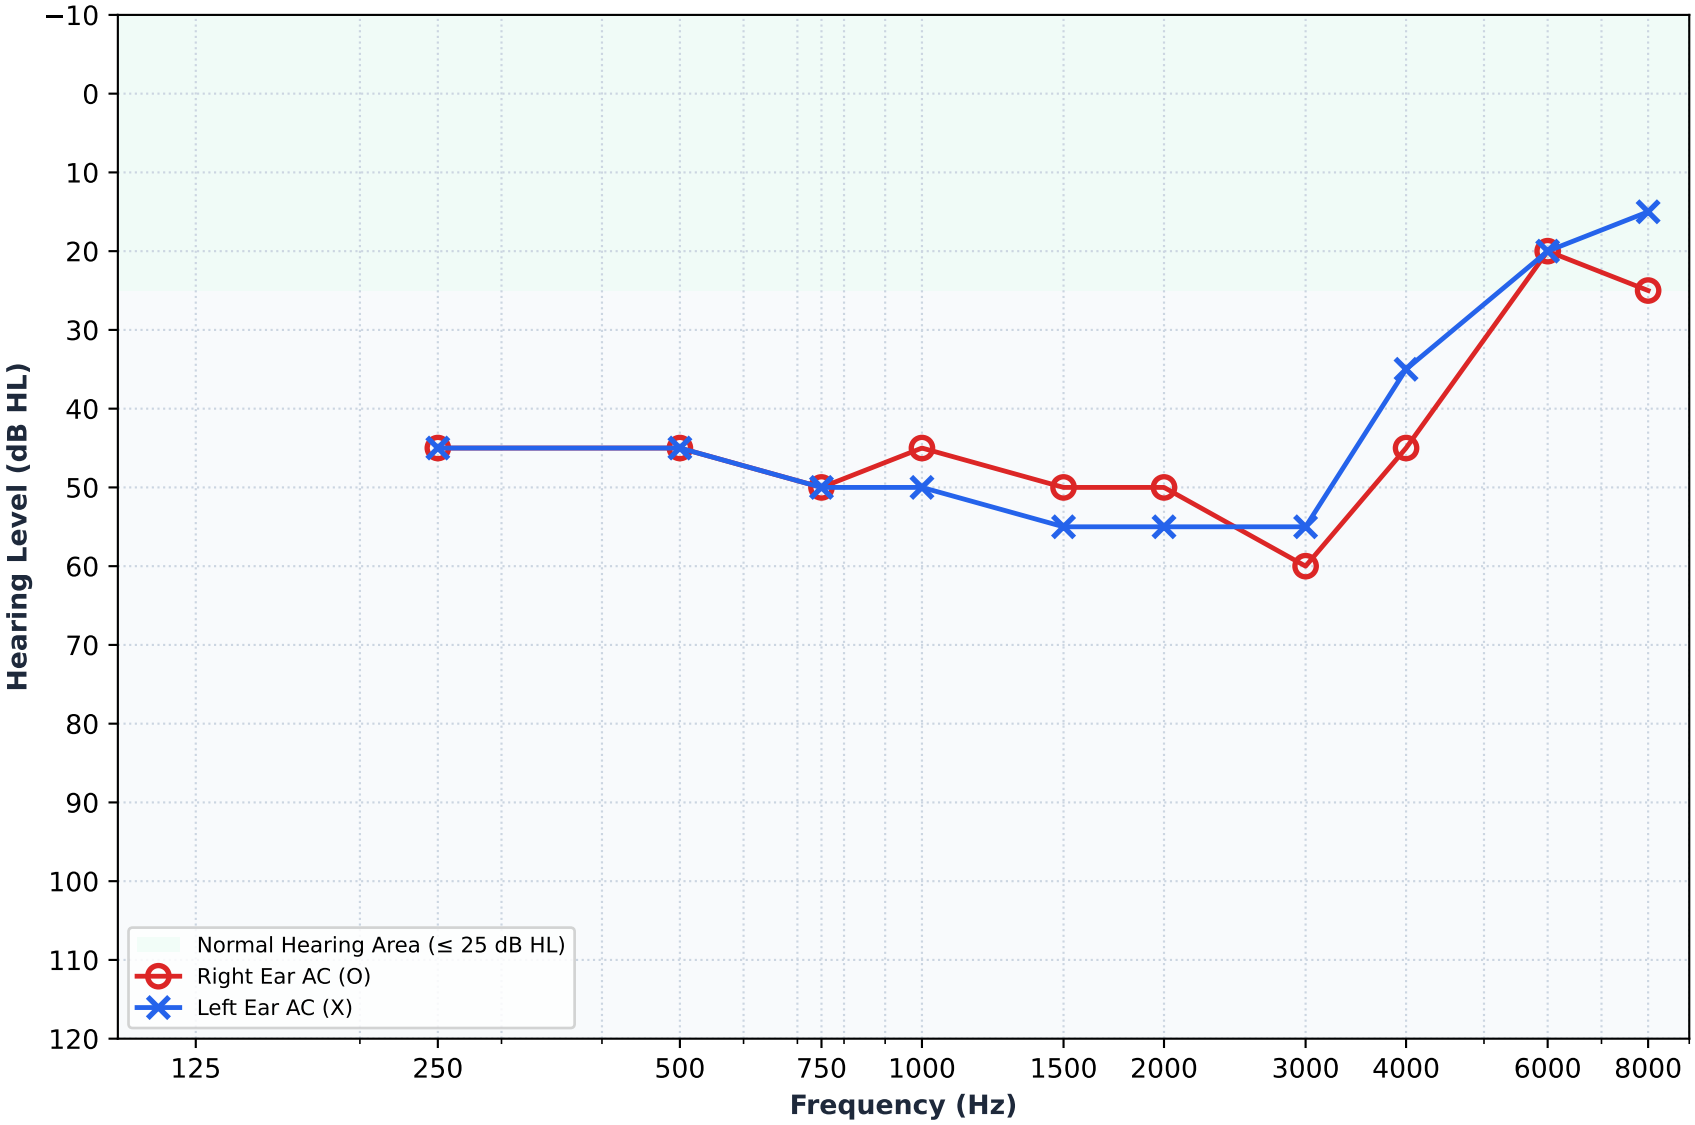


| Freq (Hz) | 125 | 250 | 500 | 750 | 1000 | 1500 | 2000 | 3000 | 4000 | 6000 | 8000 | PTA (4F) |
|---|---|---|---|---|---|---|---|---|---|---|---|---|
| Right AC (dB | - | 45 | 45 | 50 | 45 | 50 | 50 | 60 | 45 | 20 | 25 | 46.2 dB |
| Left AC (dB) | - | 45 | 45 | 50 | 50 | 55 | 55 | 55 | 35 | 20 | 15 | 46.2 dB |
| Right BC (dB | - | - | - | - | - | - | - | - | - | - | - | - |
| Left BC (dB) | - | - | - | - | - | - | - | - | - | - | - | - |

SPEECH AUDIOMETRY SUMMARY
- Right Ear: SRT = None dB HL | WRS = None%
- Left Ear:  SRT = 15.0 dB HL | WRS = None%
- Test Materials: Spondee & Phonetically Balanced Word Lists

RELIABILITY & QUALITY ASSURANCE
- Patient Reliability Score: 100.0%
- Ambient Room Noise Level: 40.20000076293945 dB SPL (ISO 8253-1 Permissible)
- Transducer Output Check: Digital Safety Limit Active (0 dBFS Clamping)

⚠ AC-ONLY INFERENCE — Approximate. Confirm with BC testing if available.
Diagnostic Classification: UNCERTAIN — REFER FOR BC TESTING (Certainty: 52.2%)
Clinical Recommendation: Ambiguous air-conduction configuration. Diagnostic certainty below threshold (<70%). Refer for bone-conduction audiometry.
Model Architecture: Random Forest Ensemble (AC_Only_Inference_v1) | Offline Local Inference