AUDIOLOGICAL EVALUATION & CLINICAL PATHOLOGY REPORT
Hardware-Grade Diagnostic Software Audiometer | ISO 8253-1 Compliant

Patient ID: PT-2026-001
Name: Ramesh Kumar
Age: 48 years
Date / Time: 2026-10-14T14:30

Clinician / Operator: Dr. S. Sharma, Au.D.
Transducer Profile: Sennheiser_HDA200
Calibration Status: Calibrated (ISO 389-1)
Deployment: Rural Tele-Audiology Field Unit

PURE TONE AUDIOGRAM (BINAURAL)

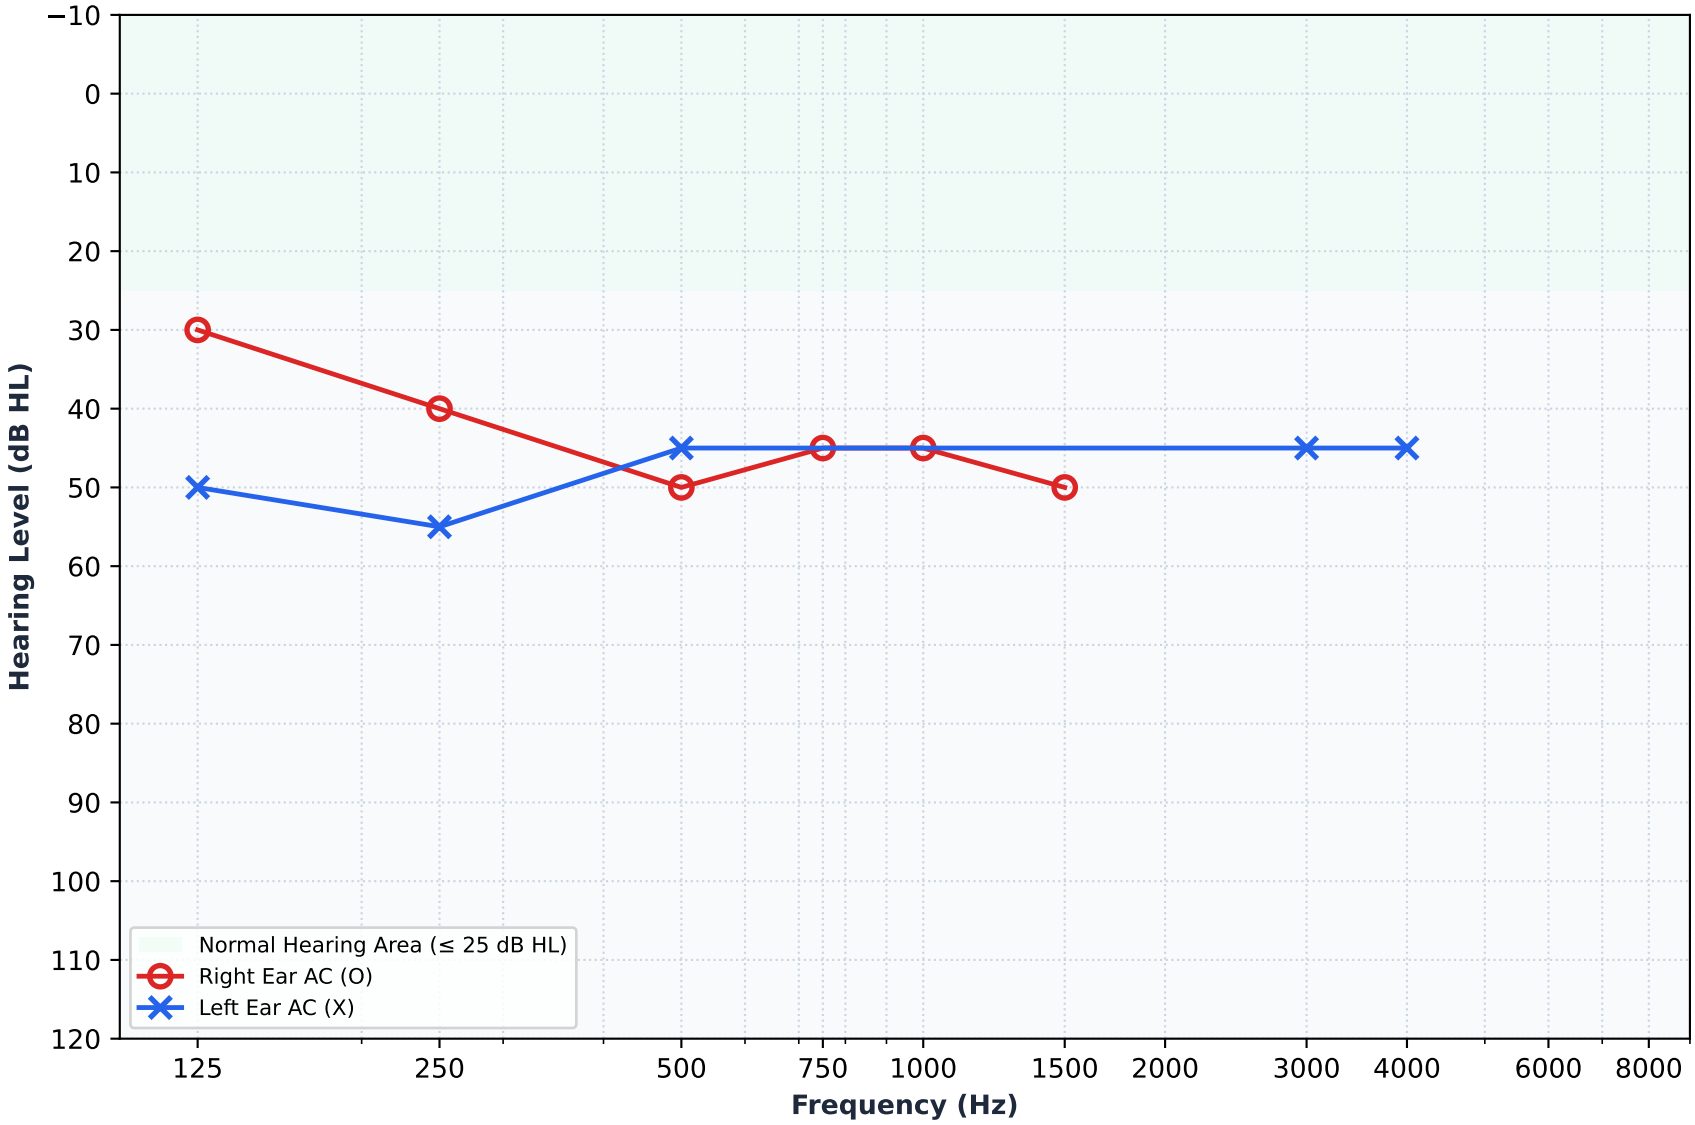

Freq (Hz)	125	250	500	750	1000	1500	2000	3000	4000	6000	8000	PTA (4F)
Right AC (dB	30	40	50	45	45	50	-	-	-	-	-	47.5 dB
Left AC (dB)	50	55	45	-	-	-	-	45	45	-	-	45.0 dB
Right BC (dB	-	-	-	-	-	-	-	-	-	-	-	-
Left BC (dB)	-	-	-	-	-	-	-	-	-	-	-	-

SPEECH AUDIOMETRY SUMMARY
- Right Ear: SRT = None dB HL | WRS = None%
- Left Ear: SRT = None dB HL | WRS = None%
- Test Materials: Spondee & Phonetically Balanced Word Lists

RELIABILITY & QUALITY ASSURANCE
- Patient Reliability Score: 100.0%
- Ambient Room Noise Level: 55.79999923706055 dB SPL (ISO 8253-1 Permissible)
- Transducer Output Check: Digital Safety Limit Active (0 dBFS Clamping)

⚠ AC-ONLY INFERENCE — Approximate. Confirm with BC testing if available.
Diagnostic Classification: UNCERTAIN — REFER FOR BC TESTING (Certainty: 37.5%)
Clinical Recommendation: Ambiguous air-conduction configuration. Diagnostic certainty below threshold (<70%). Refer for bone-conduction audiometry.
Model Architecture: Random Forest Ensemble (AC_Only_Inference_v1) | Offline Local Inference