


BioSignal Analytics Pro v1.0


ECG Analysis Report

Metric	Result
File	ecg_patient_001.csv
Samples	2500
Sampling frequency	250.00 Hz
Recording duration	10.00 s
Detected beats	12
Average BPM	72.52
Minimum BPM	70.42
Maximum BPM	74.26
Mean RR interval	0.83 s
SDNN	14.91 ms
RMSSD	18.63 ms
Dominant frequency	3.60 Hz
Signal quality	Acceptable

ECG Signal

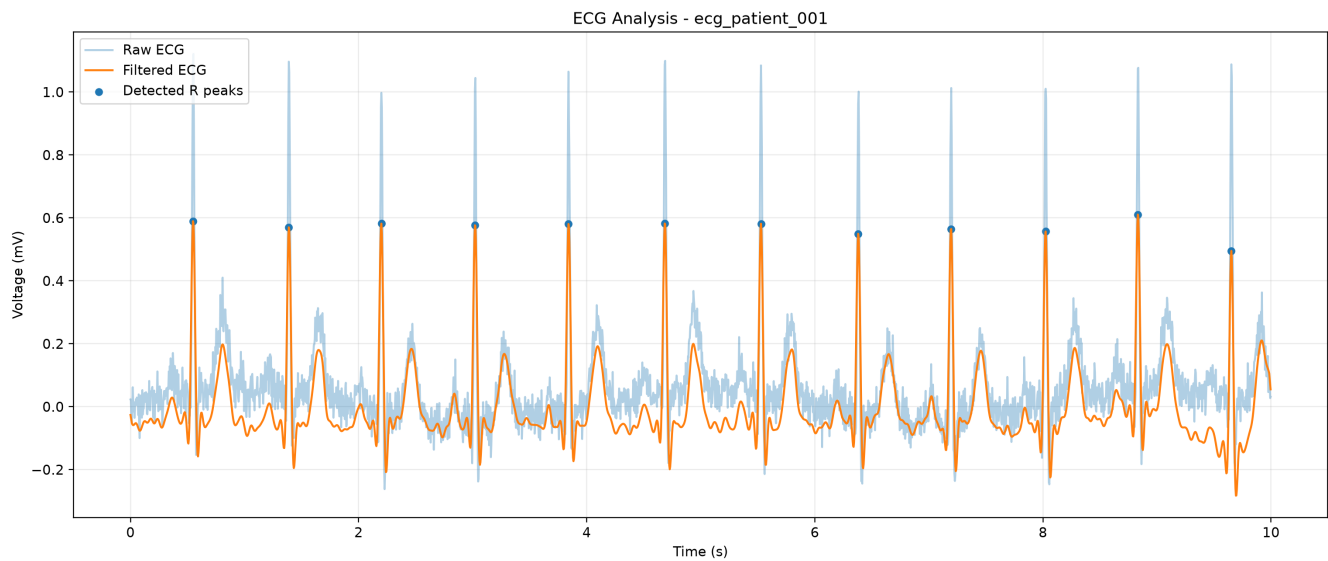

Frequency Spectrum

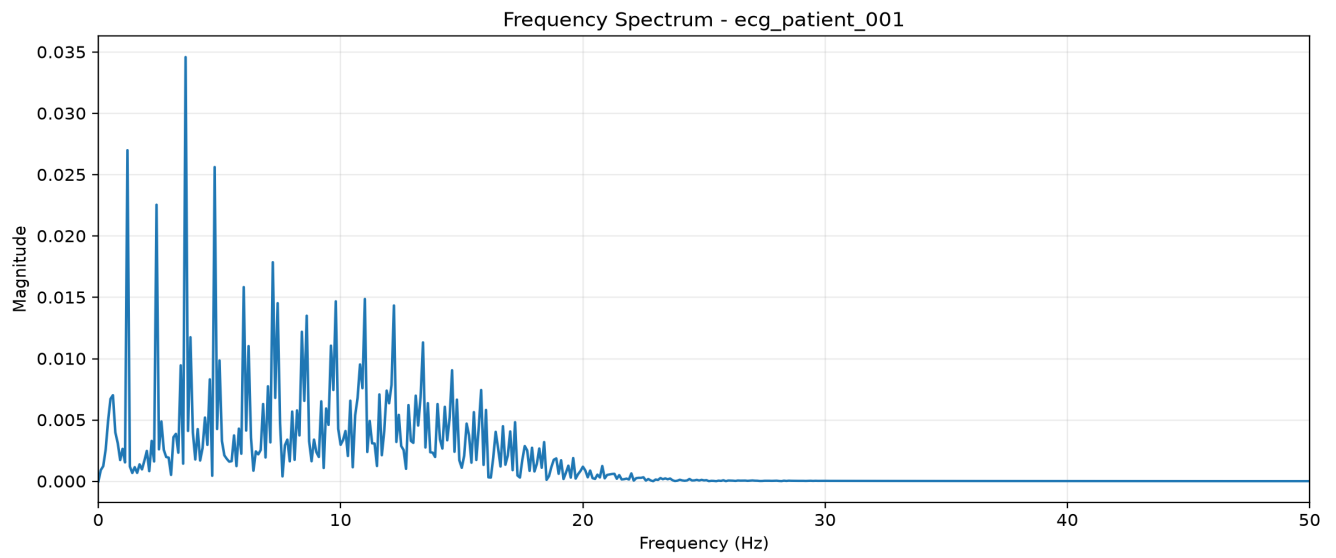

Disclaimer: This software is an educational portfolio project and is not a validated clinical diagnostic device. Results must not be used for medical decisions.