


LoTEM SENSOR CALIBRATION

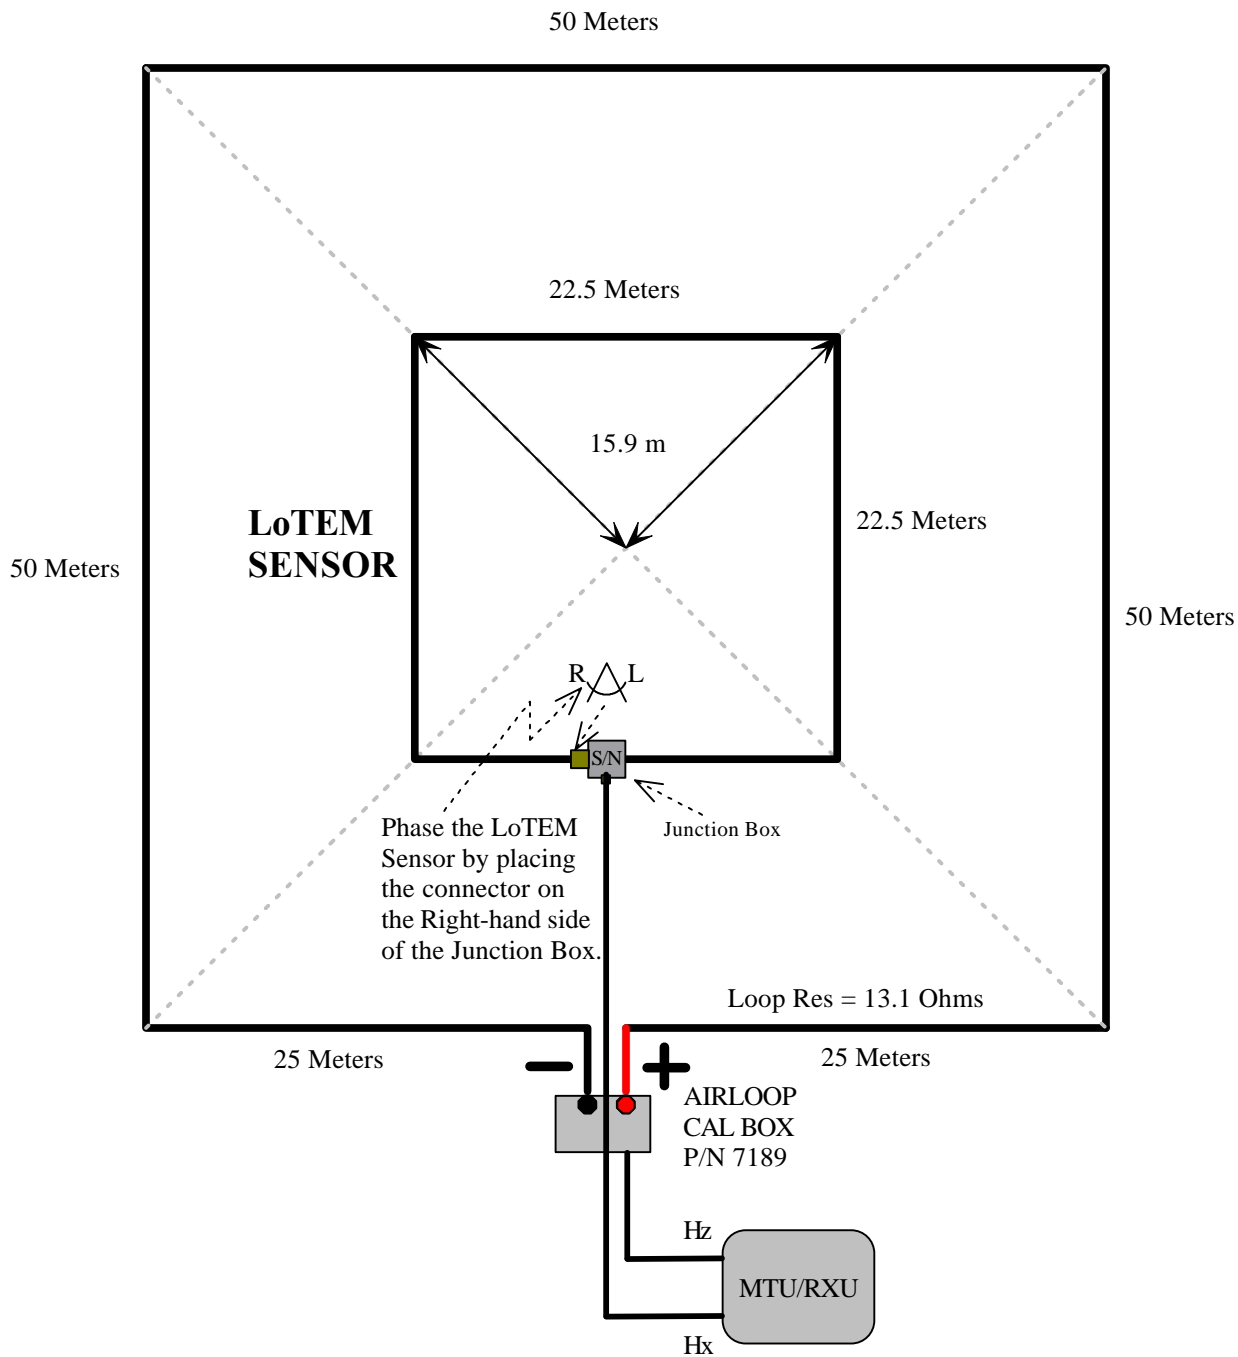

The LoTEM sensor can be calibrated with any of the PHOENIX System 2000 Receivers. Use the Off-Line WinHost Table Editor for MTU or MTU-A equipment or the V8 and RXU Startup.tbl Editor for the V-8/RXU equipment to set the following parameters in the STARTUP.TBL file or use the On-Line Parameter Table editor.

CCMN 0.0
HAMP -0.235

CCMX 0.0
HNOM 50

CPHC 0.0
HxSN TDEMssss