

Patient: GSR42 NOFILTER,

Date of Birth: Apr 12, 1953

Gender: Male

Patient ID: GSR42



Halifax Vision Centre

7105 Chebucto Road, Suite 353, Halifax, NS B3L 4W8



OS Single Field Analysis

Central 24-2 Threshold Test


Fixation Monitor: Gaze/Blind Spot
Fixation Target: Central
Fixation Losses: 4/14 XX
False POS Errors: 0%
False NEG Errors: 0%
Test Duration: 05:37
Fovea: Off

Stimulus: III, White
Background: 31.5 asb
Strategy: SITA Standard
Pupil Diameter: 1.0
Visual Acuity: 1.0
Rx: +1.00 DS

Date: Jun 15, 2023
Time: 9:31 AM
Age: 70

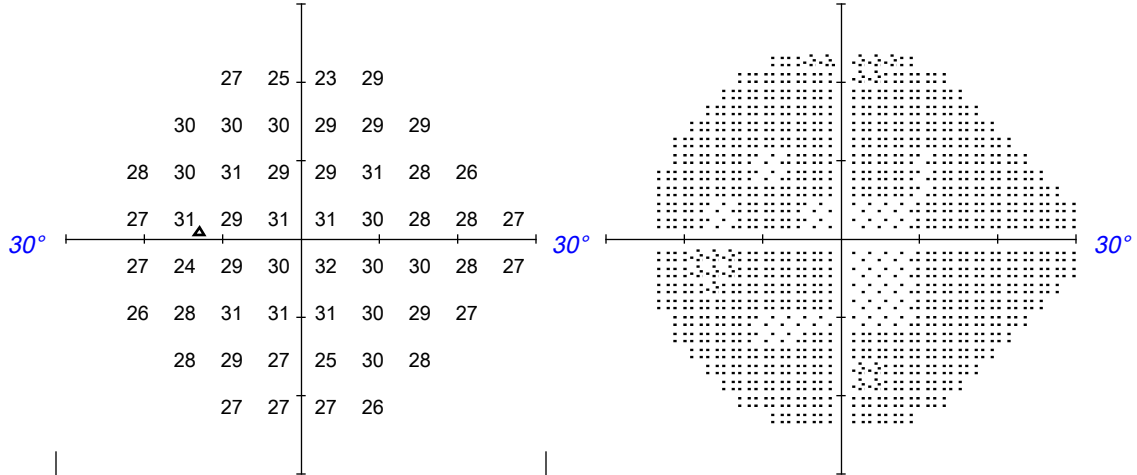

Total Deviation



Pattern Deviation

GHT: Within Normal Limits

VFI: 99%
MD24-2: -0.94 dB
PSD24-2: 1.57 dB

*** Low Test Reliability ***

:: P < 5%
::: P < 2%
::: P < 1%
::: P < 0.5%



Comments

Signature

