

Patient: **nofilter GSR20,**  
Date of Birth: **Jul 29, 1945**  
Gender: **Other**  
Patient ID: **1945.0729.AF19.E095.6239.A681**



Halifax Vision Centre  
7105 Chebucto Road, Suite 353, Halifax, NS B3L 4W8


## OS Single Field Analysis

## Central 24-2 Threshold Test

Fixation Monitor: **Gaze/Blind Spot**  
Fixation Target: **Central**  
Fixation Losses: **14/14 XX**  
False POS Errors: **17% XX**  
False NEG Errors: **19%**  
Test Duration: **09:59**  
Fovea: **Off**

Stimulus: **III, White**  
Background: **31.5 asb**  
Strategy: **SITA Standard**  
Pupil Diameter: **6.66**  
Visual Acuity: **0.666**  
Rx: **+2.25 DS**

Date: **May 24, 2023**  
Time: **10:30 AM**  
Age: **77**


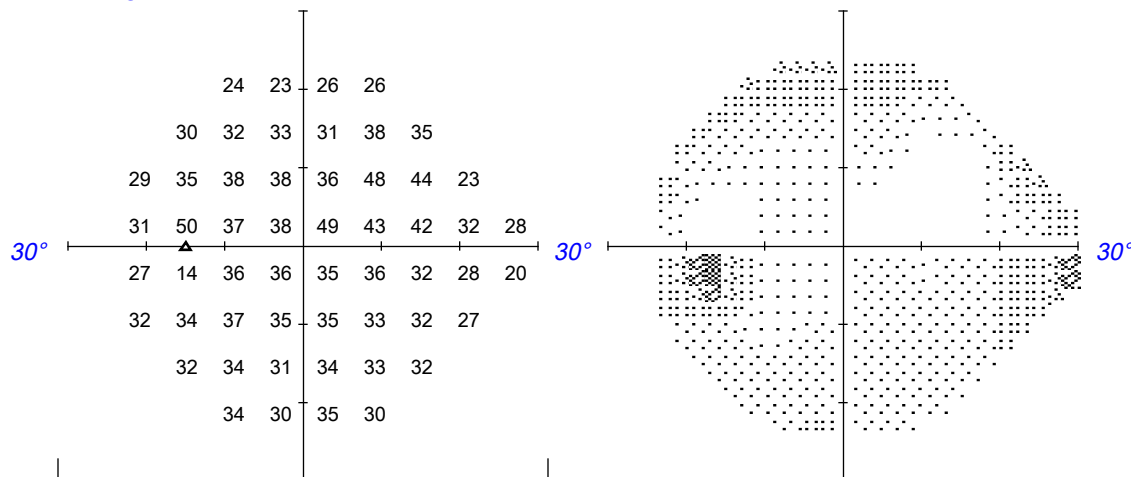


0	-2	1	1
4	4	5	3
2	7	9	8
3	7	7	18
-1	5	5	3
3	5	7	4
3	4	1	4
5	1	6	2

Total Deviation

-9	-11	-8	-8
-5	-4	-4	-5
-6	-1	0	0
-6	-1	-1	10
-10	-3	-4	-5
-5	-4	-2	-5
-5	-4	-8	-5
-3	-8	-2	-6

Pattern Deviation

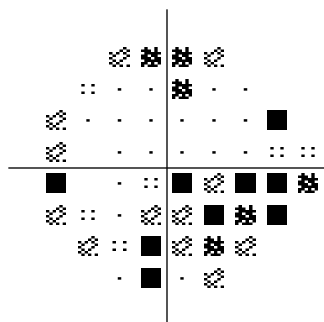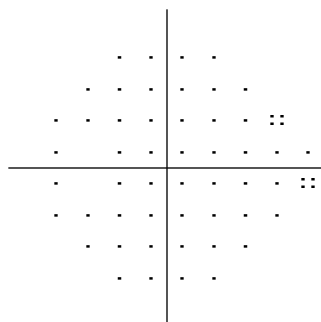

GHT: **Abnormally High Sensitivity**  
VFI: **94%**  
MD24-2: **5.14 dB**  
PSD24-2: **5.10 dB P < 0.5%**

\*\*\* Excessive High False Positives \*\*\*

:: P < 5%  
:: P < 2%  
:: P < 1%  
■ P < 0.5%



Comments

Signature

