Gender: Male

Patient ID: 1945.0729.AF19.E095.6239.A681



Halifax Vision Centre

X 7105 Chebucto Road, Suite 353, Halifax, NS B3L 4W8

OD Single Field Analysis

Central 24-2 Threshold Test

Date:

Aug 24, 2023

10:12 AM

78

Fixation Monitor: Gaze/Blind Spot
Fixation Target: Central
Fixation Losses: 8/16 XX
False POS Errors: 4%
False NEG Errors: 10%
Test Duration: 07:08


Stimulus:
Background:
Strategy:
Pupil Diameter:
Visual Acuity:
Rx: +3.00 DS


III, White 31.5 asb SITA Standard


0.4


sb Time: standard Age:

Fovea: Off

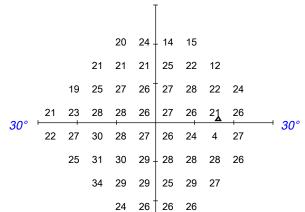











VFI: 92%

MD24-2: -3.36 dB P < 2% PSD24-2: 2.93 dB P < 2%

Total Deviation





*** Low Test Reliability ***

:: P < 5%☆ P < 2%Þ P < 1%■ P < 0.5%

Comments

Signature



© Carl Zeiss Meditec Inc., 2017. All rights reserved.