Gender: **Male**Patient ID: **GSR11**



Halifax Vision Centre

X 7105 Chebucto Road, Suite 353, Halifax, NS B3L 4W8

OD Single Field Analysis

Central 24-2 Threshold Test

Fixation Monitor: Blind Spot
Fixation Target: Central
Fixation Losses: 8/14 XX
False POS Errors: 5%
False NEG Errors: 2%
Test Duration: 05:43


Stimulus: III, White
Background: 31.5 asb
Strategy: SITA Standard


Date: Nov 28, 2022 Time: 1:46 AM Age: 68


Pupil Diameter:

Visual Acuity: 0.5 Rx: +1.00 DS +2.00 DC X 93

Fovea: Off

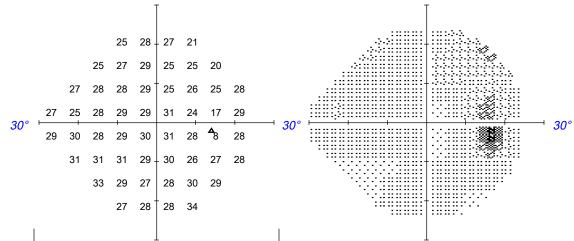









VFI: 95%

MD24-2: -1.78 dB P < 10% PSD24-2: 2.38 dB P < 5%

Total Deviation





*** Low Test Reliability ***

:: P < 5%∴ P < 2%Þ P < 1%□ P < 0.5%

Comments

Signature



© Carl Zeiss Meditec Inc., 2017. All rights reserved.