




a Independent-unit support

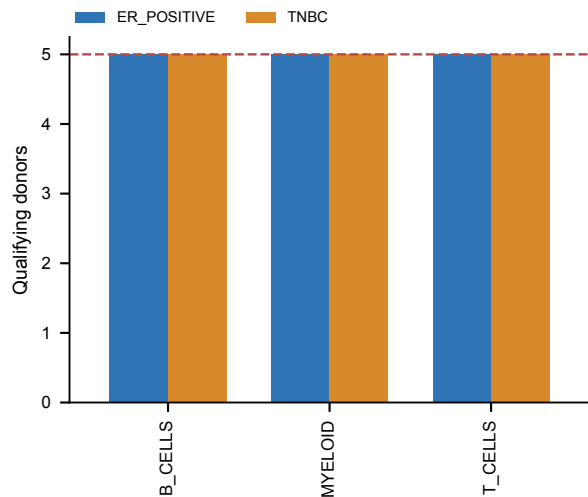

b Leave-one-donor-out diagnostics

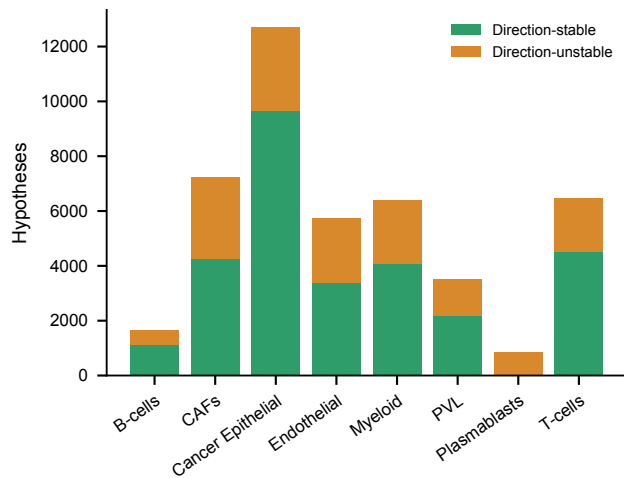

c Calibration-label composition

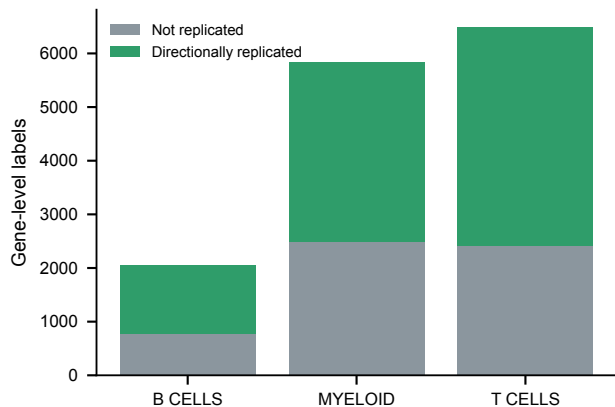

d Target-support floor

