SEA regression report summary

Sample ID
ITO-20-glass-□□□- 1

Details	
Software and regression log	
Software about	Semilab - Spectroscopic Ellipsometry Analyzer - SEA
Software version	1.8.0.4
Officially licensed to	Linyang Jiangsu
Operator	operator
Date and time of regression	07-04-2026 17:00
Comments	

Layer structure	
Overview	

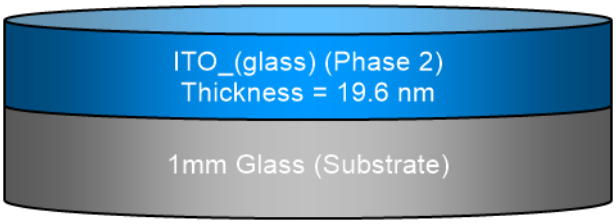

Optical model	
Phase 2	ITO_(glass)
Dispersion law	Cauchy
	Lorentz

Regression results

Measurement information				
Measurement file path	C:\Users\jijun.zhang\Desktop\□□□□□□\ ITO-20-glass-□□□-1.smdx			
Angle of Incidence	64.6°			
Regression details				
Regression 1 (EllipsoReflectance)				
Wavelength range	290.61 - 899.93 nm			
Angle of Incidence	64.6°			
Fit to	Ψ, Δ			
Angular Aperture	0°			
Fit algorithm	LMA			
Results				
Parameters	Value	Fitted	2 σ confidence limit	Unit
Model				
AOI Shift	0			°
Angular Aperture	0			°
Phase 2 (ITO_(glass))				
Thickness	19.595	X	0.033848	nm
B (µm^2)	0.046758			µm^2
C (µm^4)	1.706E-09			µm^4
D	0.055902			
E (µm^2)	-0.077691			µm^2
F (µm^4)	0.0022355	X	1.7982E-05	µm^4
f	2.04999			
E0 (eV)	4.68503			eV
Γ (eV)	1.89563	X	0.001484	eV
Eps_inf	0.15227			
N_inf	1.15106			
Derived parameters	Value			
Phase 2 (ITO_(glass))				
n @ 632.8 nm	2.0323			
k @ 632.8 nm	0.0428			
Substrate (1mm Glass)				
n @ 632.8 nm	1.4987			
k @ 632.8 nm	0.0143			
Fit quality				
R^2	0.99496			
RMSE	0.05936			

Regression graphs

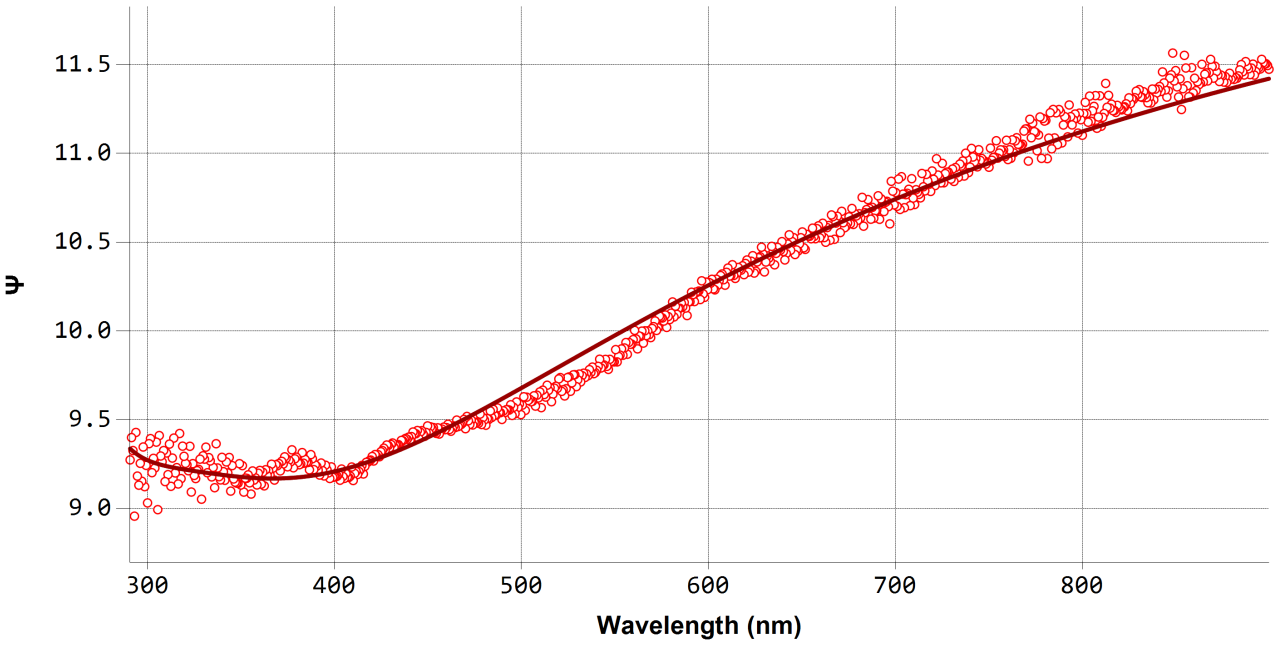

—	ITO-20-glass-□□□- 1 Measured	—	ITO-20-glass-□□□- 1 Fit

Regression graphs

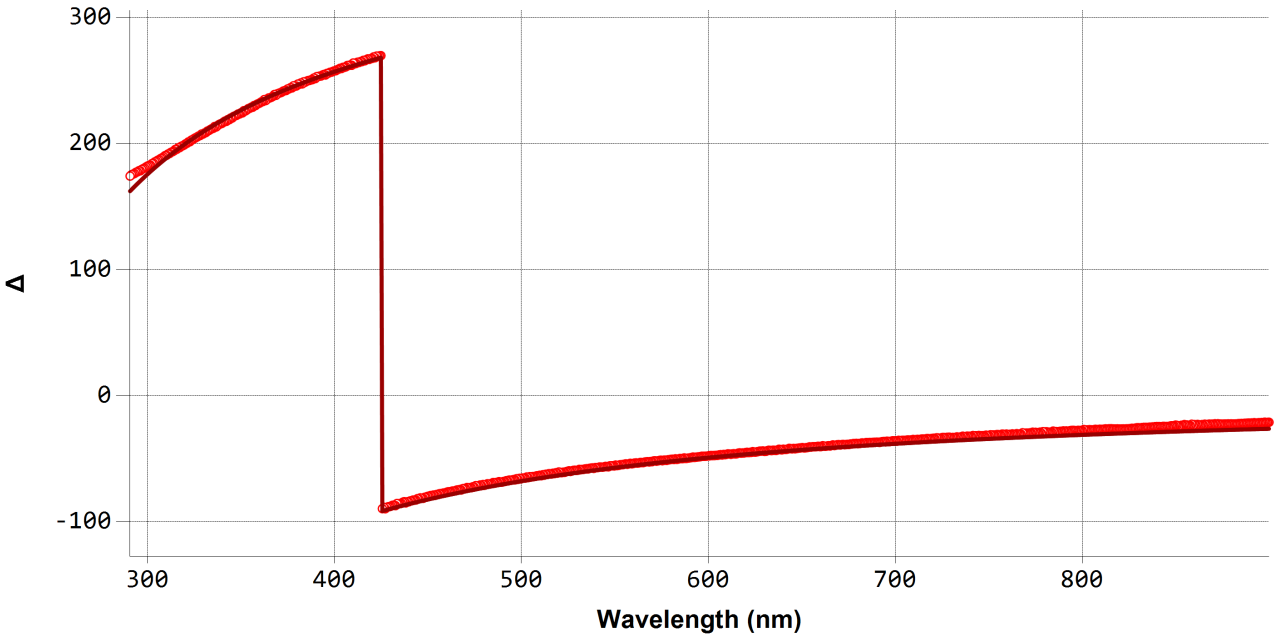

—	ITO-20-glass-□□□- 1 Measured	—	ITO-20-glass-□□□- 1 Fit

Phase 2 (ITO_(glass)) - Dispersion graphs

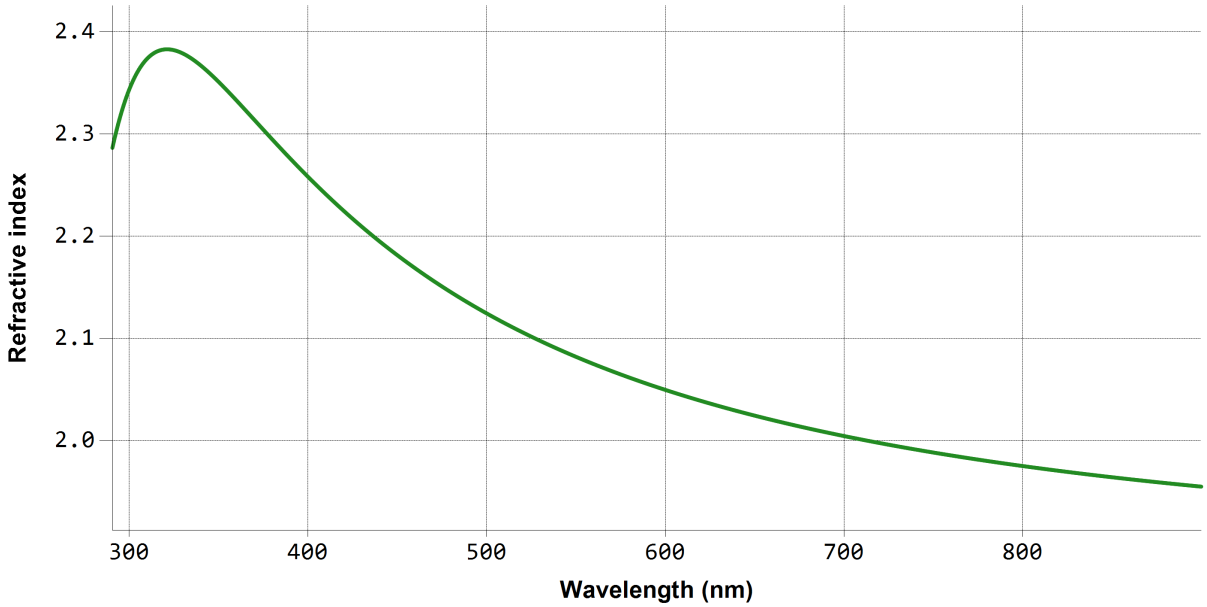

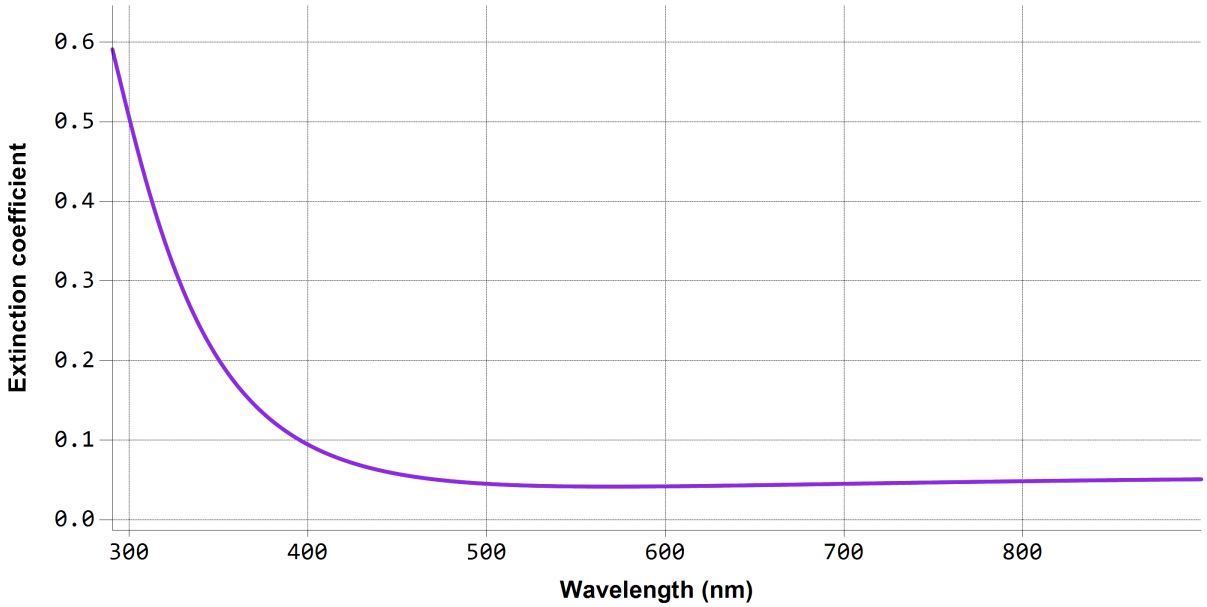

Substrate (1mm Glass) - Dispersion graphs

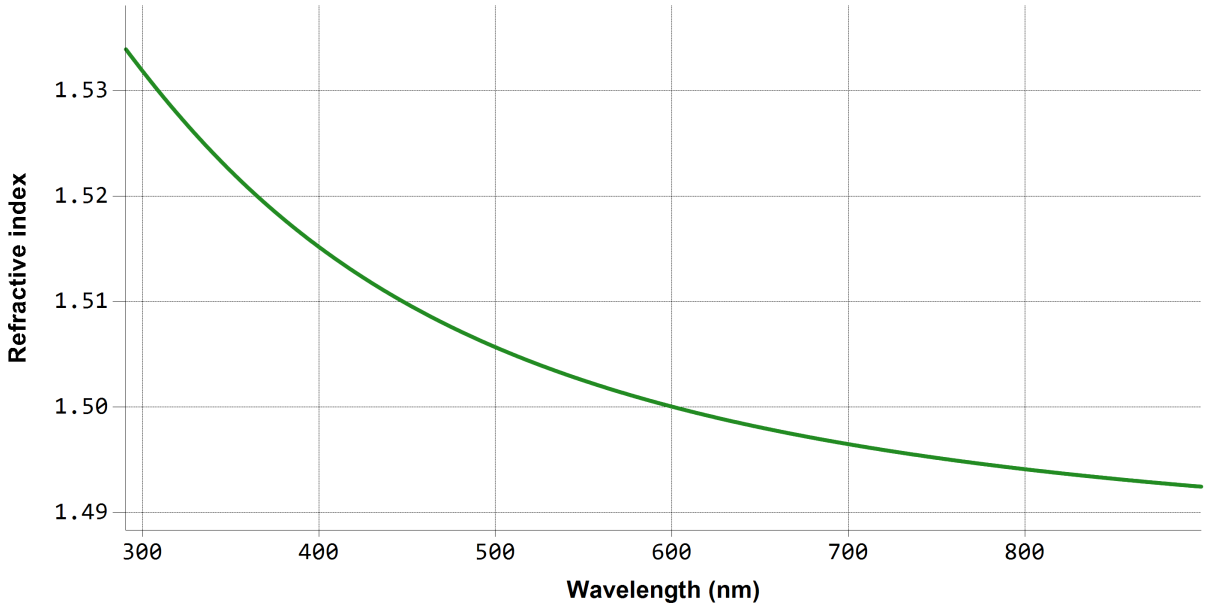

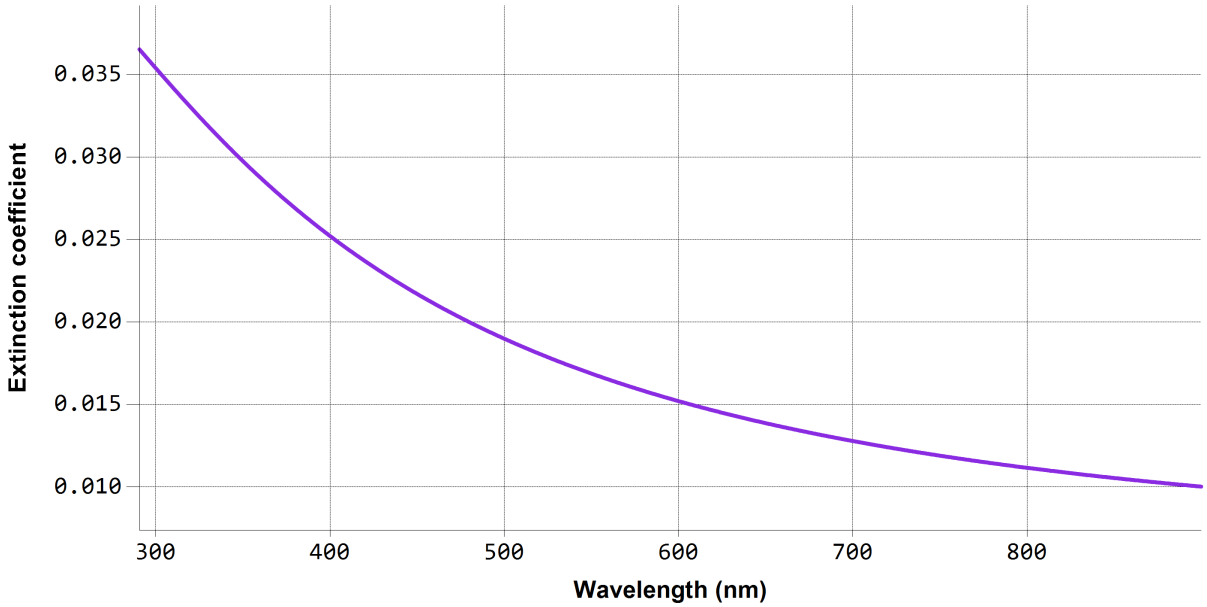

Correlation coefficients			
	Ph2 - ITO_(glass) - Thickness	Ph2 - Cauchy[1] - F (µm^4)	Ph2 - Lorentz[2] - Γ (eV)
Ph2 - ITO_(glass) - Thickness	1	-0.6271	0.1973
Ph2 - Cauchy[1] - F (µm^4)		1	-0.0045
Ph2 - Lorentz[2] - Γ (eV)			1