Irradiation setup 2 (CEEC II, E004)

Date: 2025-09-29
Tags: Lauda Irradiation setup EA advanced irrad setup
Category: Equipment
Created by: Ebrahim Abedini

Table

Setup name	Irradiation set-up 2	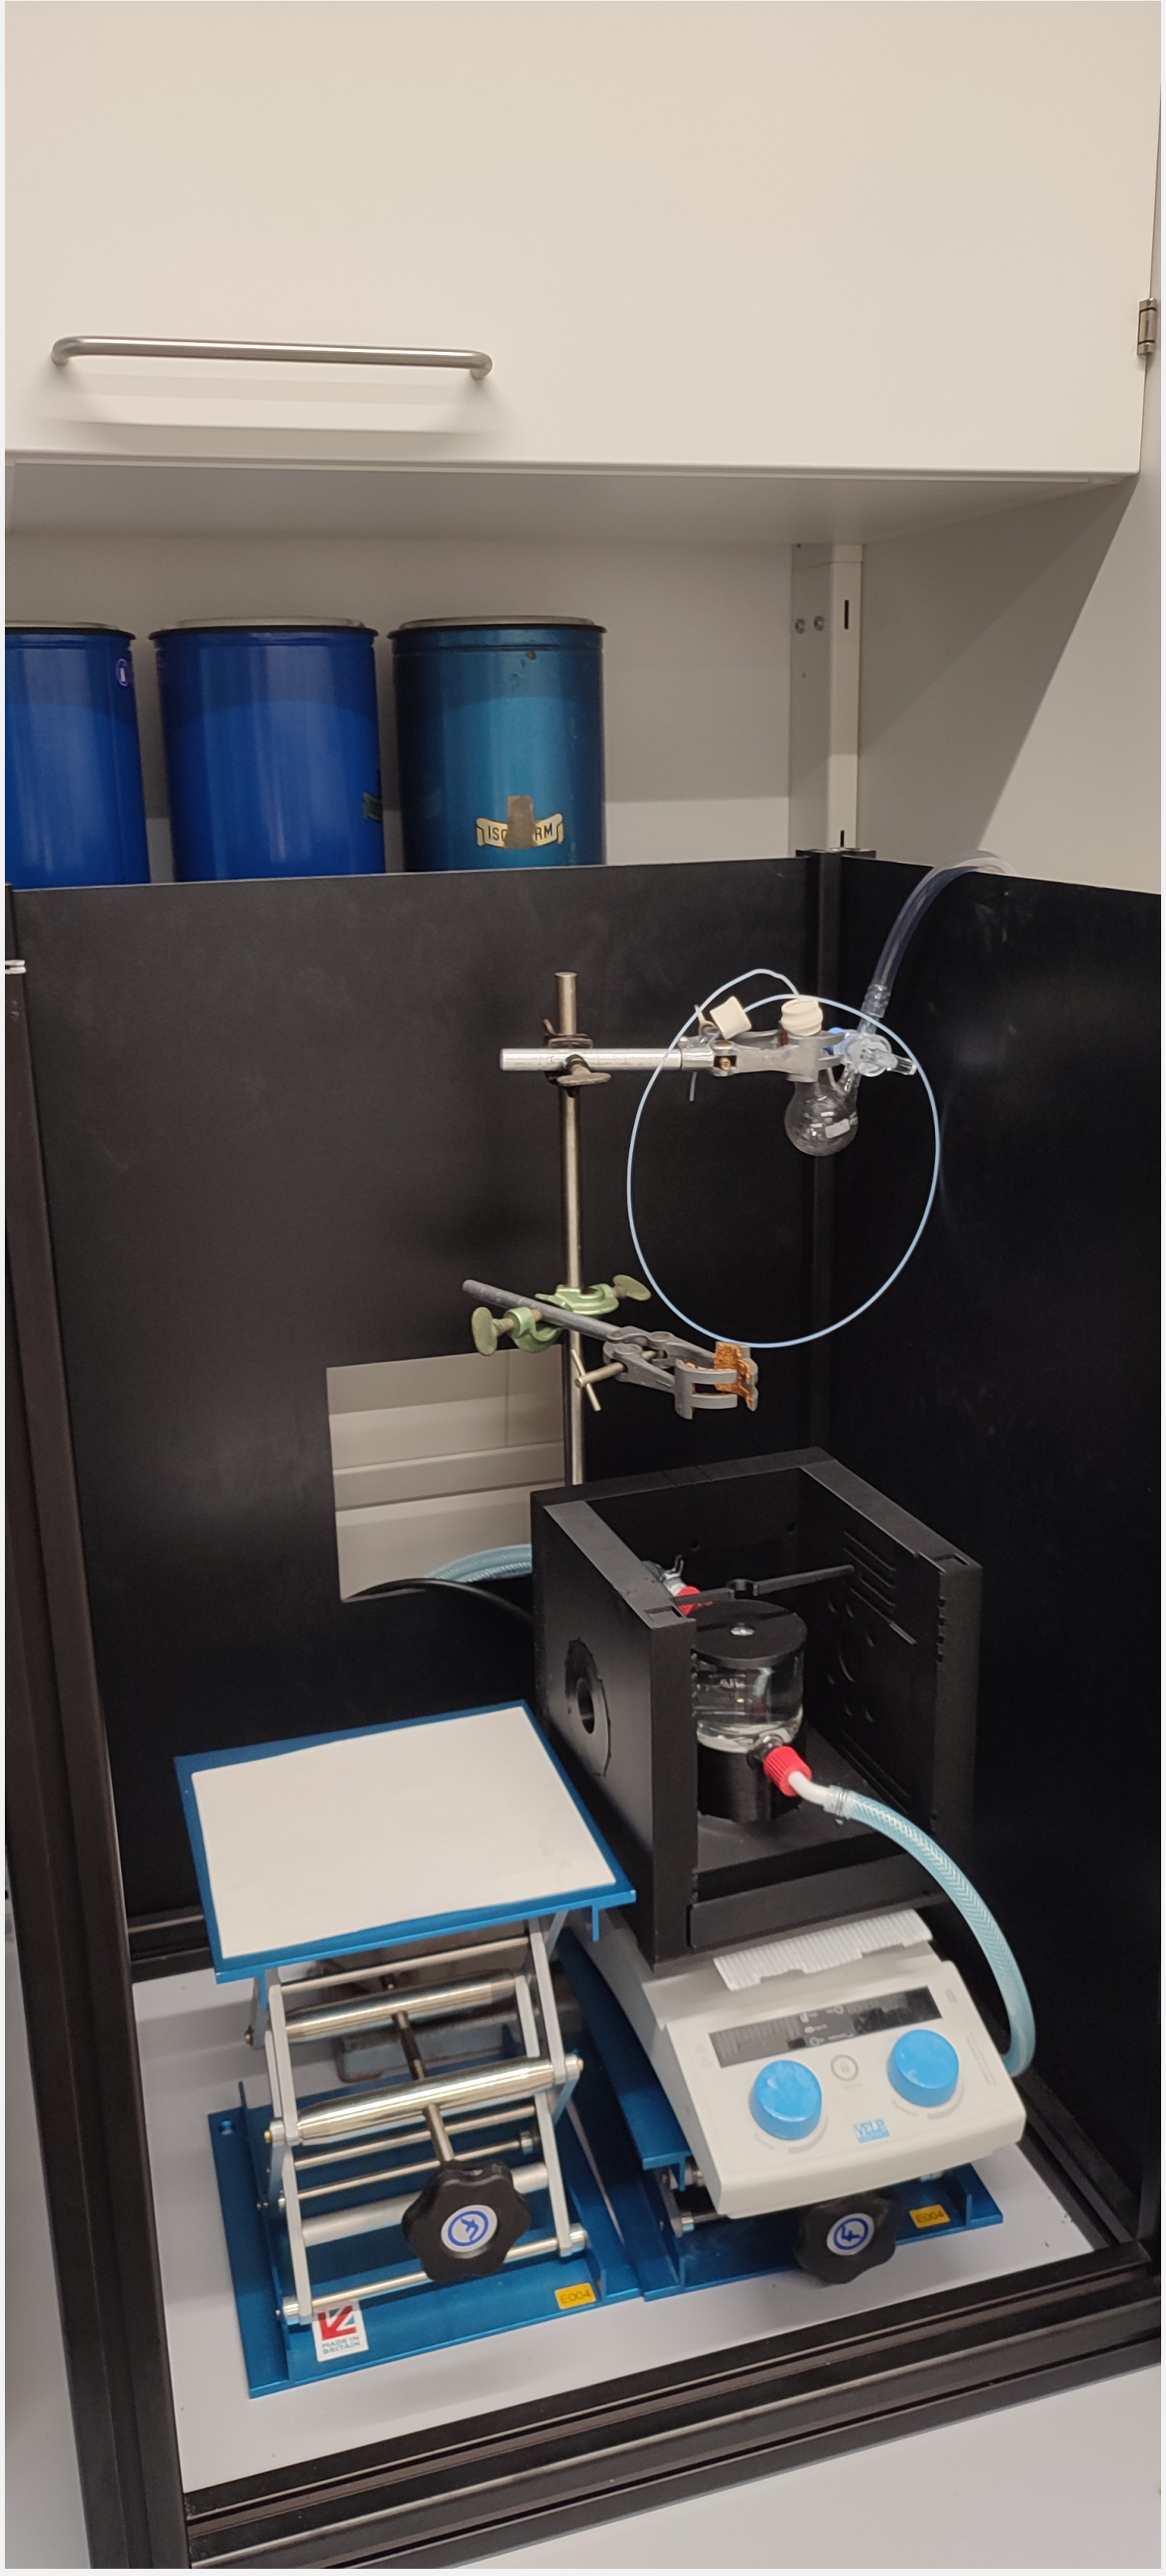

Type of the setup	Equipment - Advanced irradiation setup V1.0 I
Information	*Information - Everything about Usage of Irradiation Set-Up*
Location	CEEC II, lab E004 Right side of the lab Color: Purple
Name in Instruments Calendar	*Irradiation set-up 2*
Power sources	Power Sources - BLS-18000-1 1 Power Sources - BLS-13000-1E Power Sources - BLS-1000-2 1
LEDs	Light Source - UHP LED 6500 K (white)-1 Light Source - UHP LED 470 nm Light Source - UHP LED 365 nm-2 Light Source - HP LED 405 -1 Light Source - HP LED 6500 K (white) -1
Beam combiner	Beam Combiner - Beam Combiner LCS-BC25-0409 -1
Lauda	Equipment - Lauda - LOOP Thermoelectric thermostat, L100, 2
FireSting	Equipment - Firesting Fiber-Optic Oxygen Meter 2 Channel (Firesting 2)
Introduction	Alex, Nadja
Responsible Person	Alex, Nadja

Protocol on usage of the setup	Protocol - Irradiation setup Protocol - Catalytic tests in irradiation setup in flasks/vials Protocol - Using the advanced irradiation setup V1.0
Additional Information	***Before the LED lamps can be turned on safety precautions have to be taken! (lab coat, blue nitril gloves, UV-glasses).*** ***Check the cleanness of the Lauda's solution before starting your photocatalytic experiments.*** ***Choose the appropriate holder for your Schlenk/NMR tube.*** ***Choose the appropriate aperture for the LED configuration that you want to use.*** ***Close the dark box from all 4 sides before starting the irradiation.*** ***The switch on the LED itself should not be used (should always be in the "on" ("I") position).*** ***After usage, check the Argon flow to be closed, LEDs disconnected from the power source, and the stirring plate to be turned off.*** ***Do not use the stirring plate's heating function while there are plastic tapes on it.*** ***Clean the degassing cannula after usage. (Replace with a new one in case of usage of noble metals).***
Status from	*29/09/2025*

Linked resources

- Beam Combiner - Beam Combiner LCS-BC25-0409 -1
- Equipment - Firesting Fiber-Optic Oxygen Meter 2 Channel (Firesting 2)
- Equipment - Advanced irradiation setup V1.0 I
- Equipment - Manual irradiation setup
- Equipment - Lauda - LOOP Thermoelectric thermostat, L100, 1
- Equipment - Lauda - LOOP Thermoelectric thermostat, L100, 2
- Light Source - UHP LED 365 nm-1
- Light Source - UHP LED 470 nm-1
- Light Source - UHP LED 6500 K (white)-1
- Light Source - HP LED 405 -1
- Light Source - HP LED 6500 K (white) -1
- Light Source - UHP LED 365 nm-2
- Power Sources - BLS-1000-2 1
- Power Sources - BLS-13000-1E
- Power Sources - BLS-18000-1 1
- Protocol - Catalytic tests in irradiation setup in flasks/vials
- Protocol - Cleaning of double walled beaker

Attached file

Irradiation-setup-2.jpg
sha256: 13632ca456585577760b358d1b00437004fb3d14c29a84b87dd399881271c1c4

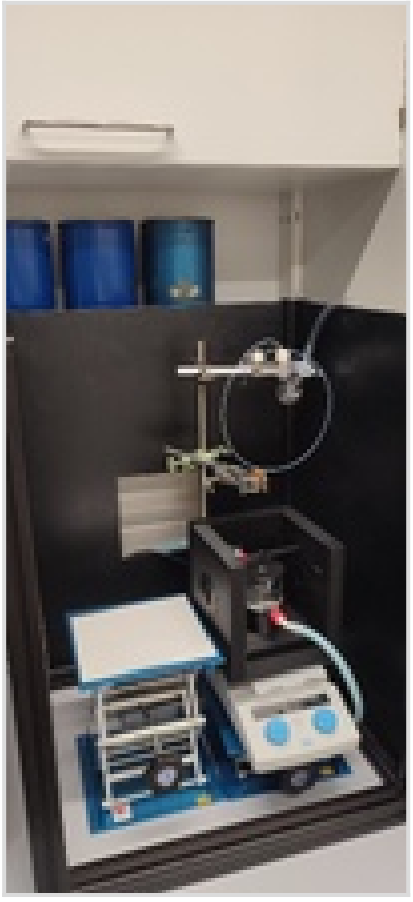

Unique eLabID: 20250929-362cacdf1e34018e126e0d4d340e4360dce2e144
Link: https://elab.water-splitting.org/database.php?mode=view&id=280