

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 1/34

| Parameters - Overview       |   | (1st interrog.) |
|-----------------------------|---|-----------------|
| Mode                        |   | VVI-CLS         |
| Basic rate/Night rate [bpm] |   | 60/-----        |
| CLS                         |   | 120             |
| Sensor/Rate fading [bpm]    |   | 120/-----       |
| Upper rate response [bpm]   |   |                 |
| Home Monitoring             |   | OFF             |
| Pulse amplitude [V]         |   | 2.4             |
| Pulse width [ms]            |   | 0.4             |
| Capture control             |   | ATM             |
| Sensitivity [mV]            |   | AUTO            |
| Refract. period [ms]        |   | 250             |
| Sensing polarity            | ⌚ | BIPL            |
| Pacing polarity             | ⌚ | BIPL            |
| Calculated ERI              |   | 11 Y. 2 Mo.     |

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 2/34

| Parameters - Bradycardia       |           | (1st interrog.) |
|--------------------------------|-----------|-----------------|
| Mode                           | VVI-CLS   |                 |
| Basic rate/Night rate [bpm]    | 60/-----  |                 |
| Basic rate [bpm]               | 60        |                 |
| Night rate [bpm]               |           |                 |
| Night begins                   |           |                 |
| Night ends                     |           |                 |
| Hysteresis [bpm]               |           |                 |
| Repetitive/Scan cycles         |           |                 |
| Magnet response                | ASync     |                 |
| CLS                            | 120       |                 |
| CLS response                   | Medium    |                 |
| CLS resting rate control [bpm] | +20       |                 |
| Vp required                    | No        |                 |
| Sensor/Rate fading [bpm]       | 120/----- |                 |
| Max. activity rate [bpm]       | 120       |                 |
| Sensor gain                    | ⌀ AUTO    |                 |
| Sensor threshold               | Medium    |                 |
| Rate fading                    |           |                 |
| Rate increase [bpm/cycle]      | 2         |                 |
| Rate decrease [bpm/cycle]      | 0.5       |                 |
| Upper rate response [bpm]      |           |                 |

| Parameters - Bradycardia    |   | (1st interrog.) |
|-----------------------------|---|-----------------|
| Pulse amplitude [V]         |   | 2.4             |
| Pulse width [ms]            |   | 0.4             |
| Capture control             |   | ATM             |
| Threshold test start [V]    |   | 2.4             |
| Safety margin [V]           |   |                 |
| Search type                 |   | Time of day     |
| Interval [h]                |   |                 |
| Time of day                 |   | 00:30           |
| Status                      |   | OK              |
| Note                        |   |                 |
| Last measured threshold [V] |   | 0.6             |
| Date                        |   | 01/10/2024      |
| Time                        |   | 00:34           |
| Sensitivity [mV]            |   | AUTO            |
| Refract. period [ms]        |   | 250             |
| Sensing polarity            | ⌚ | BIPL            |
| Pacing polarity             | ⌚ | BIPL            |
| Calculated ERI              |   | 11 Y. 2 Mo.     |

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 4/34

|                                     |                 |
|-------------------------------------|-----------------|
| <b>Parameters - Home Monitoring</b> | (1st interrog.) |
|-------------------------------------|-----------------|

|                         |  |
|-------------------------|--|
| <b>General settings</b> |  |
|-------------------------|--|

|                              |     |
|------------------------------|-----|
| PID                          | 89  |
| Home Monitoring              | OFF |
| Time of transmission [hh:mm] |     |
| High rate                    |     |
| Event-based IEGM             |     |

|                     |  |
|---------------------|--|
| <b>Last message</b> |  |
|---------------------|--|

|                    |     |
|--------------------|-----|
| Message type       | --- |
| Message created on |     |

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life

PSW 2301.A/1

Page 5/34

|                                 |                 |
|---------------------------------|-----------------|
| <b>Parameters - Diagnostics</b> | (1st interrog.) |
|---------------------------------|-----------------|

|                           |  |
|---------------------------|--|
| <b>Recording triggers</b> |  |
|---------------------------|--|

|                           |          |
|---------------------------|----------|
| High rate                 | ON       |
| Patient trigger           | OFF      |
| Pre-trigger recording [%] | 75       |
| IEGM signal               | Filtered |

|                   |  |
|-------------------|--|
| <b>Statistics</b> |  |
|-------------------|--|

|                              |       |
|------------------------------|-------|
| Start resting period [hh:mm] | 02:00 |
| Resting period duration [h]  | 4.0   |
| Thoracic impedance           | ON    |

|                  |  |
|------------------|--|
| <b>High rate</b> |  |
|------------------|--|

|                            |     |
|----------------------------|-----|
| High rate limit [bpm]      | 150 |
| High rate counter [Events] | 8   |
| Enable lead check          | ON  |



|                                |            |                             |
|--------------------------------|------------|-----------------------------|
| Parameters - Patient           |            | (1st interrog.)             |
| ID                             |            |                             |
| Last name                      | 295131-MRI |                             |
| First name                     | Chen-Yan   |                             |
| Date of birth                  | 04/25/1938 |                             |
| Gender                         | Female     |                             |
| Date of implant                | 03/24/2023 |                             |
| Hospital, City                 | CSMUH      |                             |
| Physician                      | Dr.Su      |                             |
| Phone                          |            |                             |
| Symptom                        | B2<br>B3   | Dizzy spells<br>Bradycardia |
| ECG indication                 |            |                             |
| E6 Atrial flutter/fib. + Brady |            |                             |
| Etiology                       |            |                             |
| XXX                            |            |                             |
| LVEF [%]                       |            |                             |
| XXX                            |            |                             |
| NYHA                           |            |                             |
| XXX                            |            |                             |
| Remark                         |            |                             |

Leads

| Lead model | Manufacturer | Serial number | Type | Implantation | Channels |
|------------|--------------|---------------|------|--------------|----------|
| Solia S 60 | Biotronik    | 8000717314    | BIPL | 03/24/2023   | RV       |
|            |              |               |      | XX/XX/XXXX   |          |
|            |              |               |      | XX/XX/XXXX   |          |
|            |              |               |      | XX/XX/XXXX   |          |

**Diagnostics - Timing**

(1st interrog.)

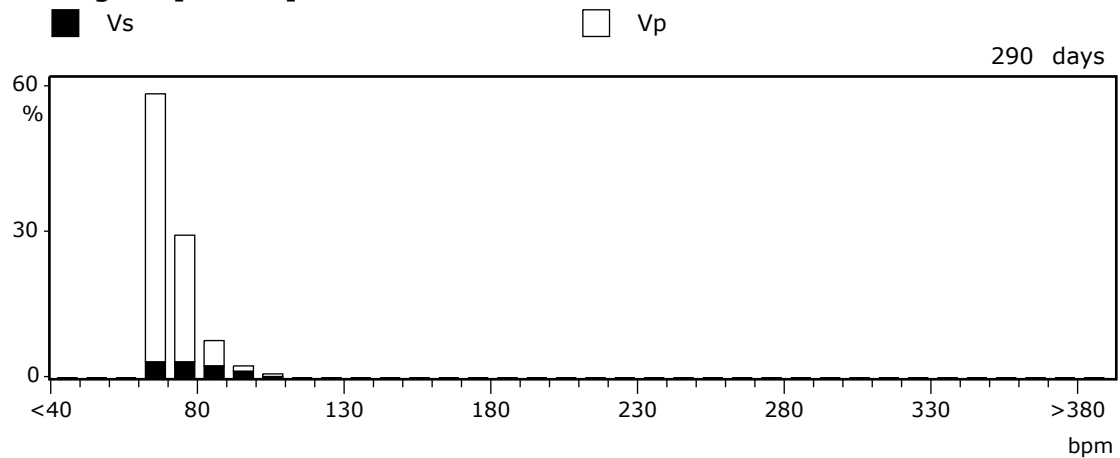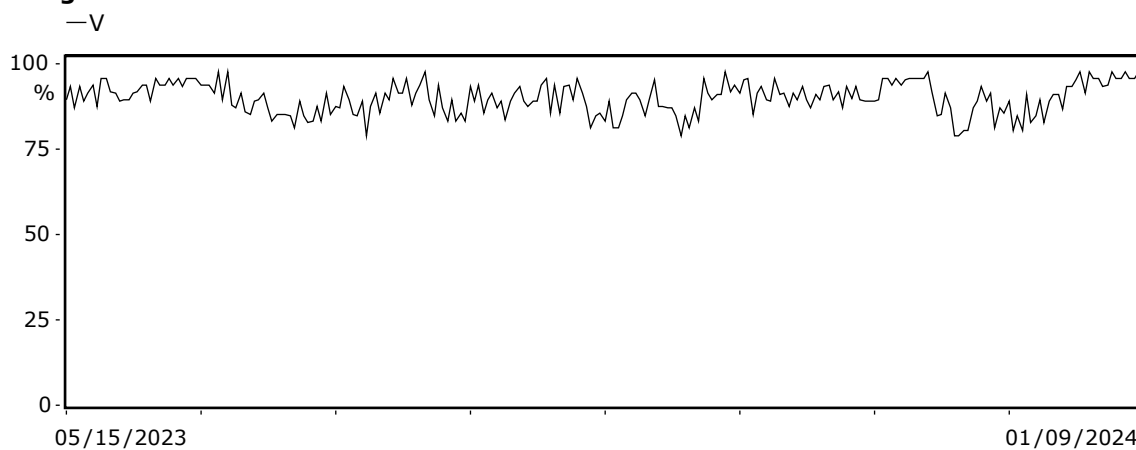
**Rate histogram [% time]****Event episodes and events****Pacing trend**

Start 03/25/2023


**Diagnostics - HF monitor**

(1st interrog.)


## Mean rate

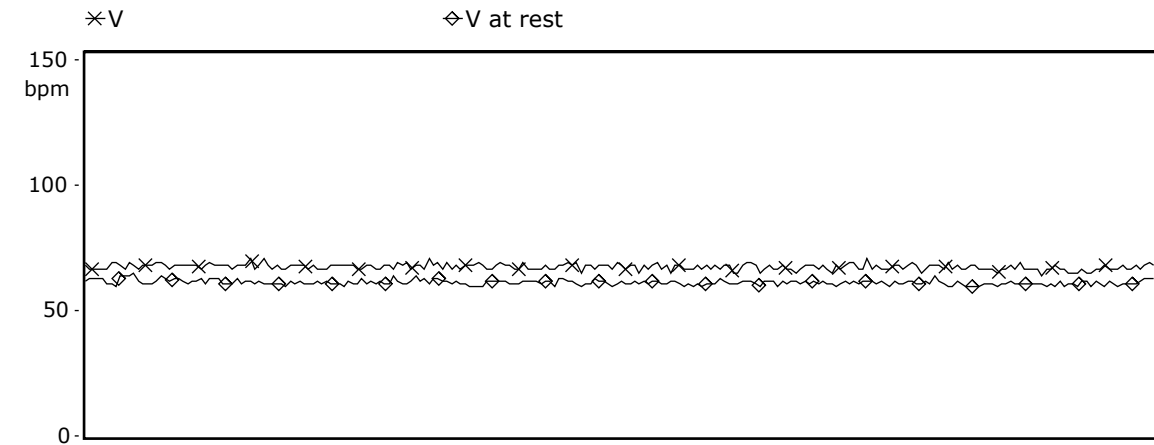

## Patient activity

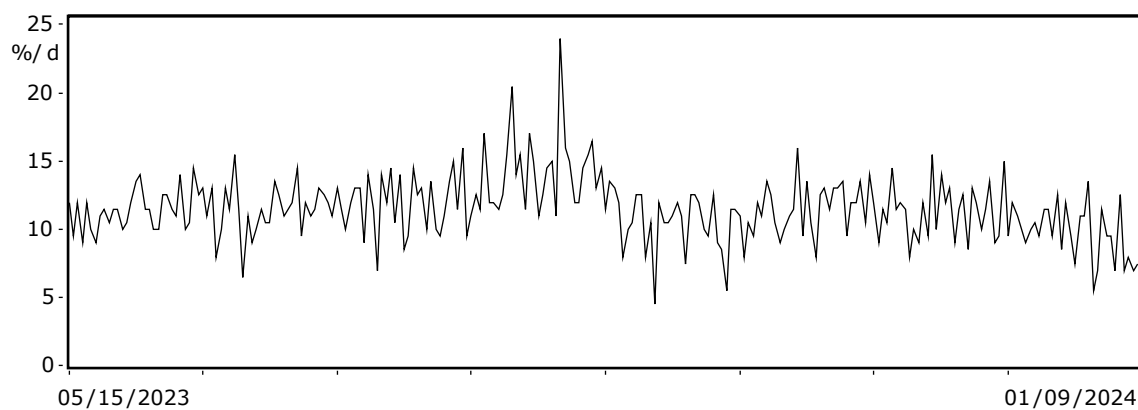

## Thoracic impedance

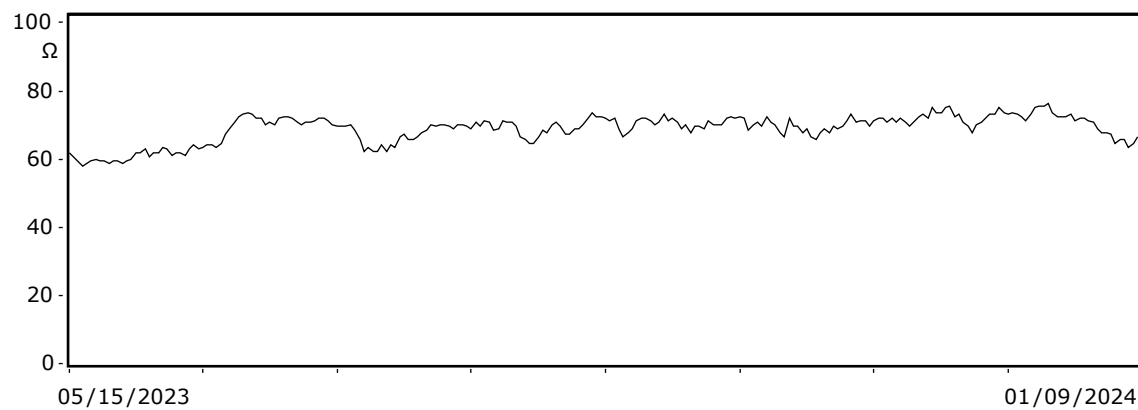


Start      03/25/2023




**Diagnostics - 24 hours**

(1st interrog.)

Rate

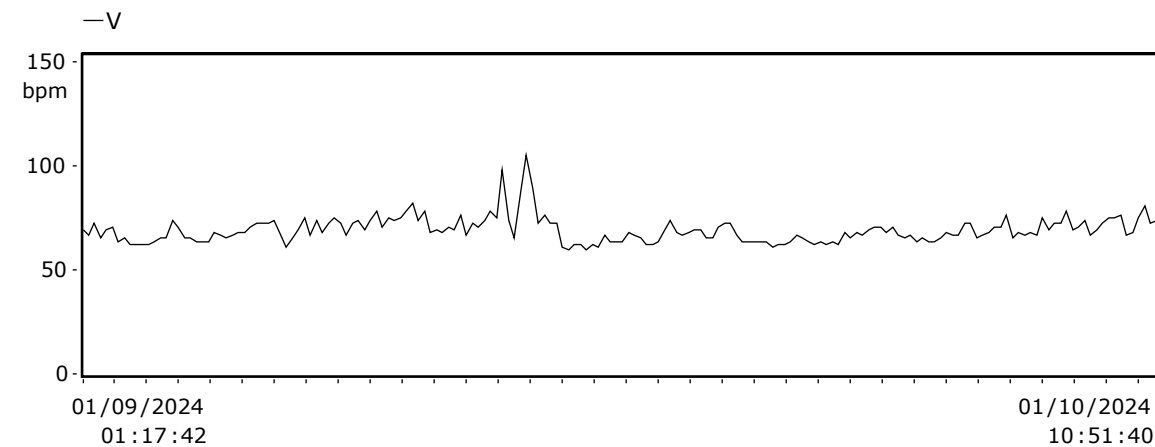

% paced

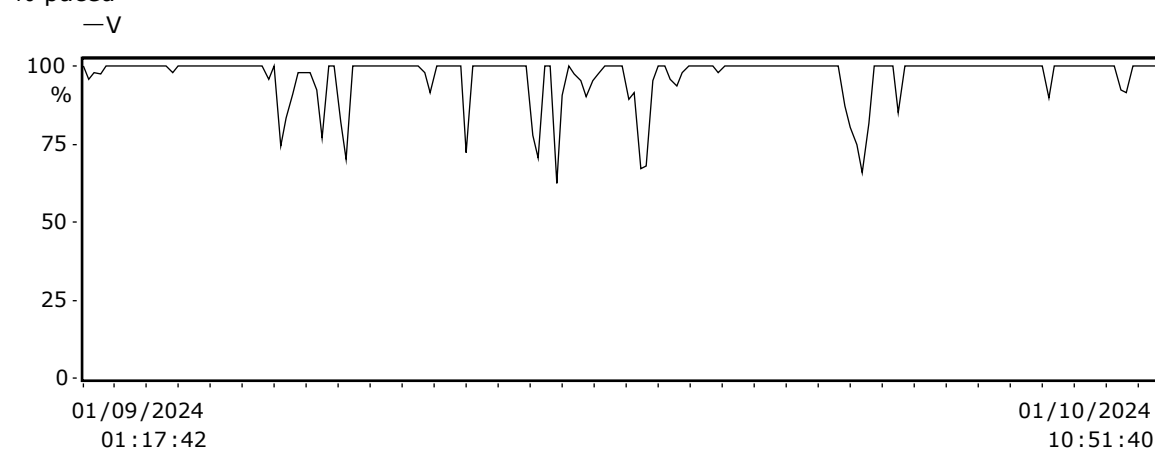


Start 03/25/2023

**Diagnostics - More diag. - Event counters**

**(1st interrog.)**

**Event counters**

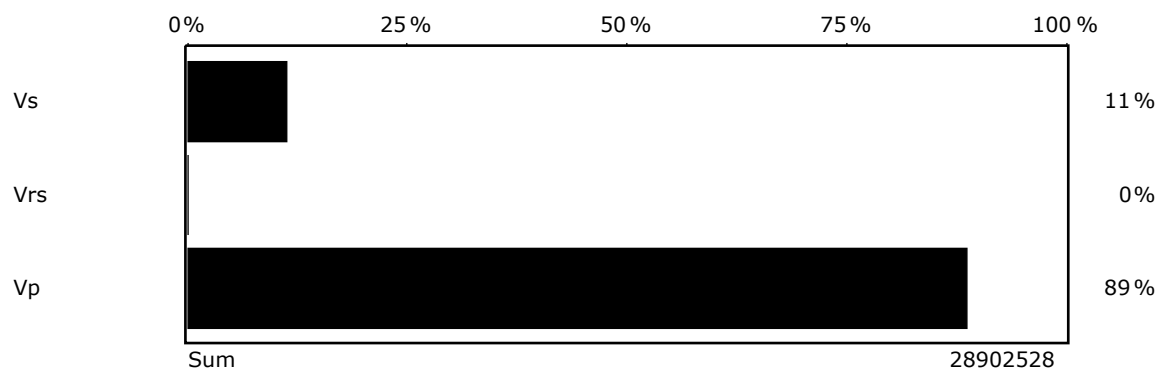

Start 03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life

PSW 2301.A/1

Page 11/34


**Diagnostics - More diag. - Pulse ampl. and threshold**

**(1st interrog.)**

Ventricle

✕ Threshold

◇ Amplitude

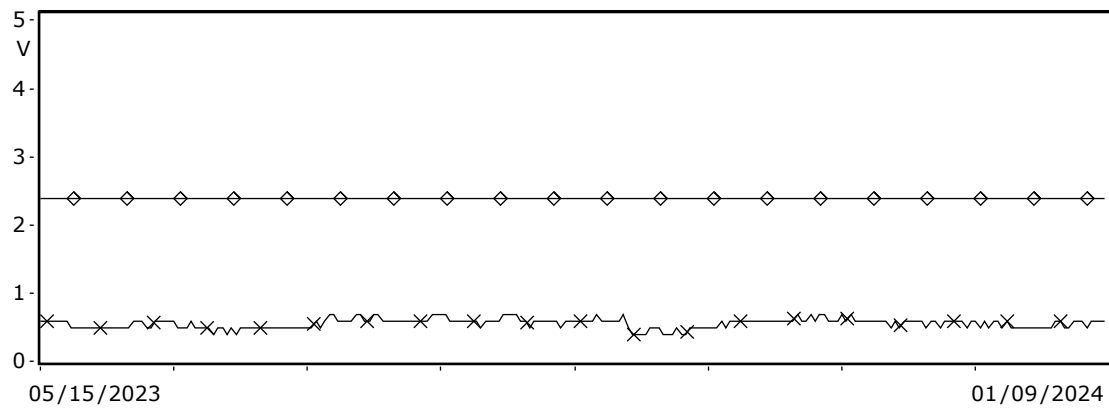

Start 03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life


PSW 2301.A/1

Page 12/34

**Diagnostics - More diag. - Sensor rate**

**(1st interrog.)**

Sensor rate [% time]

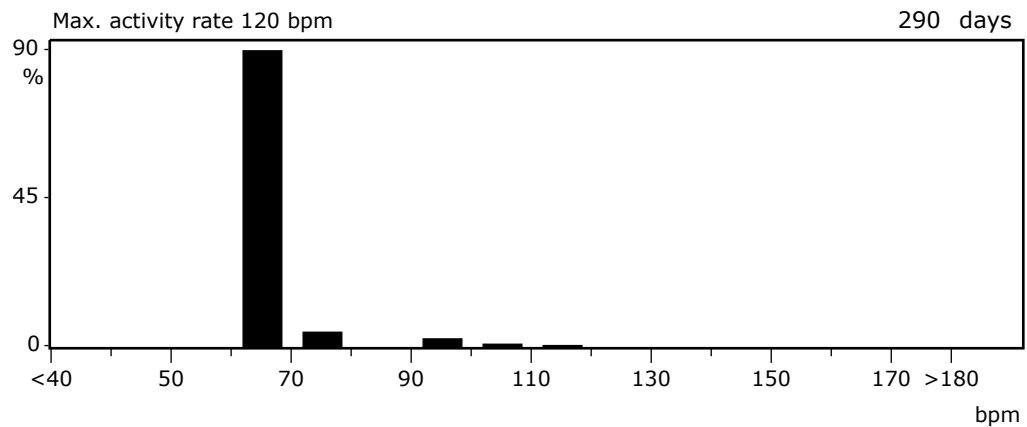

Start 03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 13/34

**Diagnostics - More diag. - Arrhythmia**

**(1st interrog.)**

**Ven. arrhythmia**

High ventricular rate episodes [Count]

0

Start      03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life

PSW 2301.A/1


Page 14/34

**Diagnostics - More diag. - P/R wave trend**

**(1st interrog.)**

P/R wave trend

—V

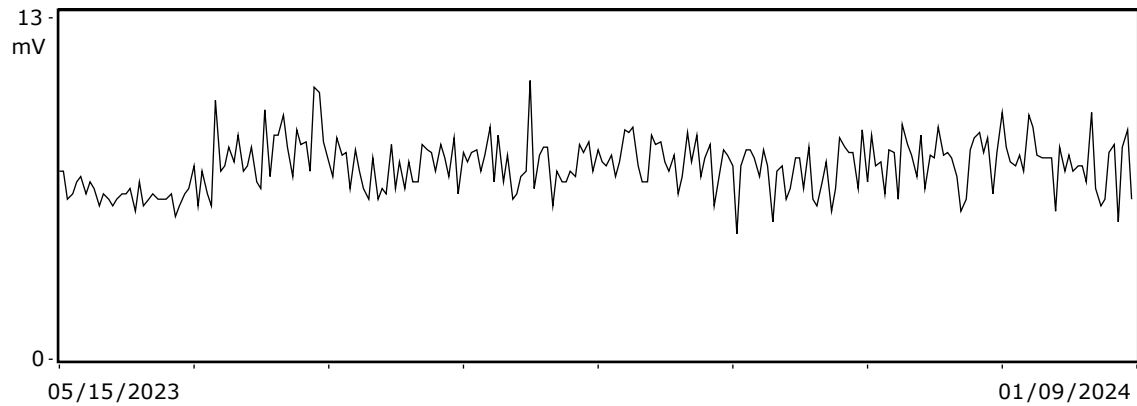

Start 03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life

PSW 2301.A/1


Page 15/34

**Diagnostics - More diag. - Lead impedance trend**

**(1st interrog.)**

Lead impedance trend

—V

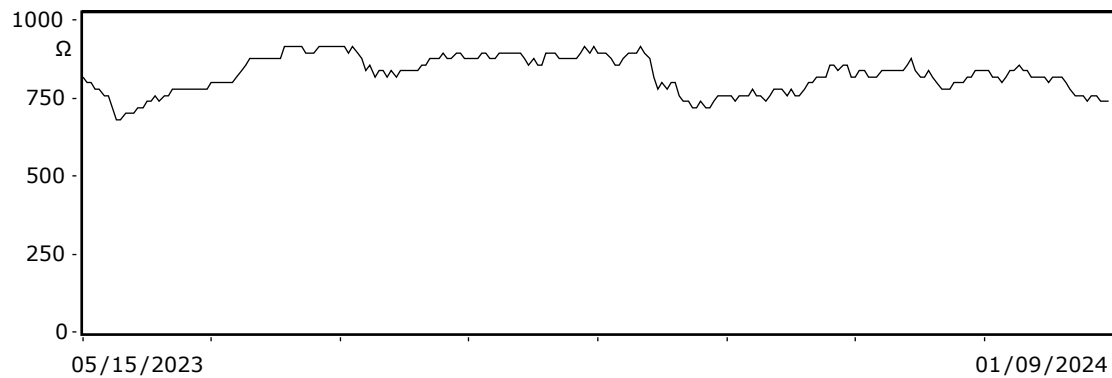


Start 03/25/2023

**Follow-up - Details**


(1st interrog.)

Rate histogram [% time]

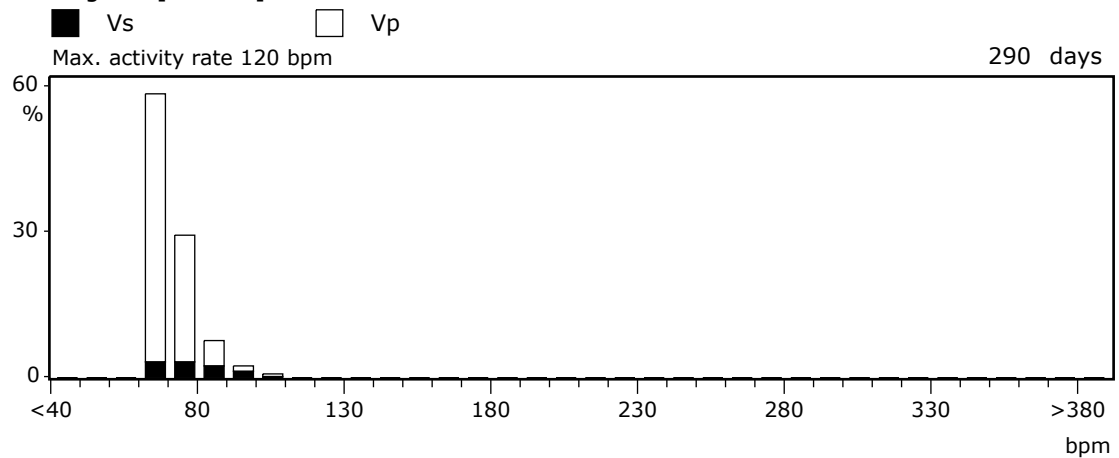


## Long-term trends

Rate

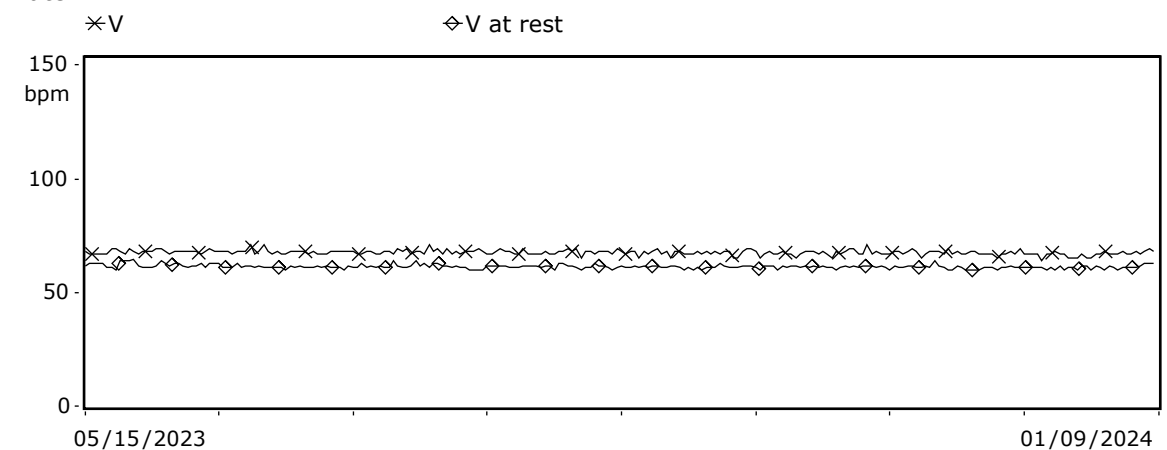

## Patient activity

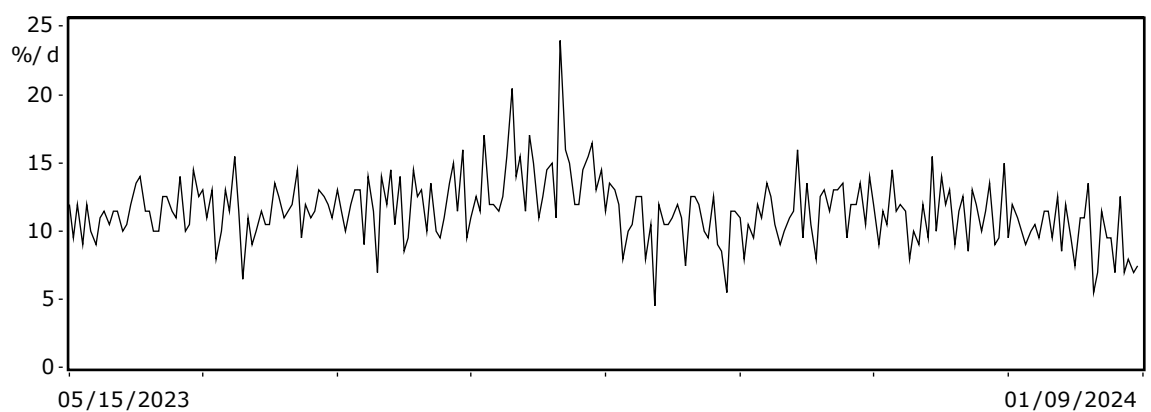

Start      03/25/2023




**TrendView**

(1st interrog.)


Mean rate

—V

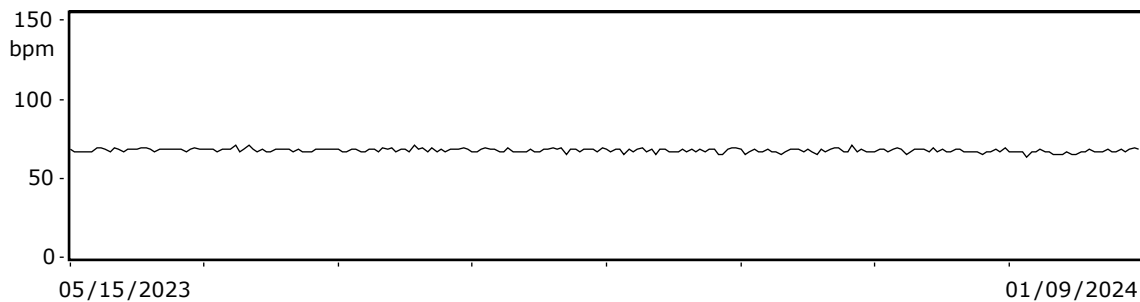


Pacing threshold

—V

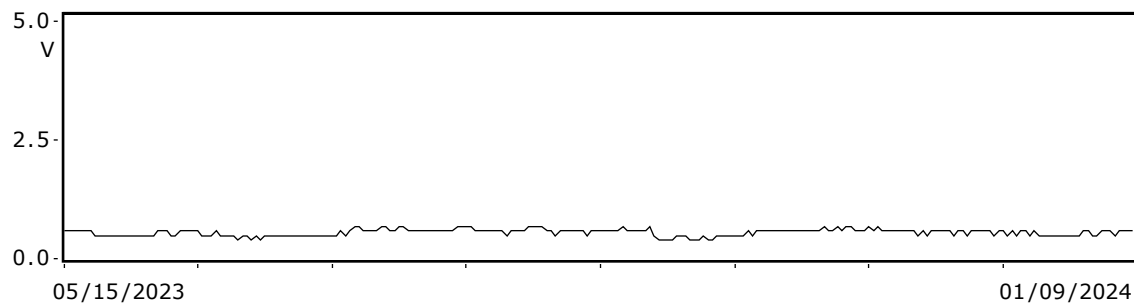


P/R wave amplitude

—V

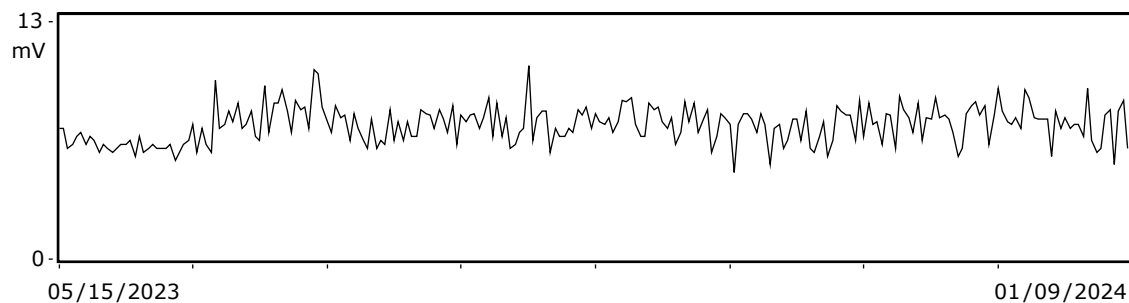

Lead impedance

—V

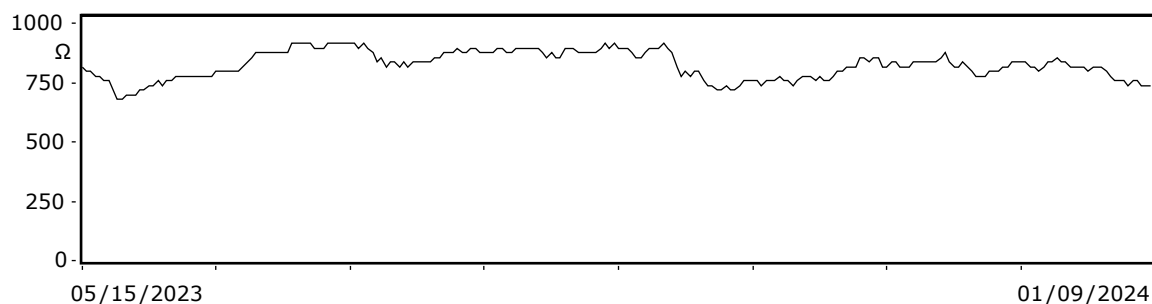

Start 03/25/2023

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 18/34



**BIOTRONIK**  
excellence for life

**TrendView**

(1st interrog.)

Pacing in V [%]

89

Start 03/25/2023

| Recordings - Episodes |      |          |         |     |    |
|-----------------------|------|----------|---------|-----|----|
| No.                   | Date | Duration | Trigger | MVR | PC |

|                  |                 |
|------------------|-----------------|
| <b>Follow-up</b> | (1st interrog.) |
|------------------|-----------------|

**Patient**

|                 |                      |
|-----------------|----------------------|
| Name            | 295131-MRI, Chen-Yan |
| Last follow-up  | 03/25/2023           |
| Date of implant | 03/24/2023           |

**Device status**

|                                |             |
|--------------------------------|-------------|
| Program count                  | 3           |
| Home Monitoring                | OFF         |
| MRI program                    | OFF         |
| Mode                           | VVI-CLS     |
| Basic rate [bpm]               | 60          |
| Pulse amplitude [V]            | 2.4         |
| Pulse width [ms]               | 0.4         |
| Expected ERI                   | 11 Y. 2 Mo. |
| Battery status                 | OK          |
| Remaining battery capacity [%] | 95          |

**Test results**

|                             |   |      |
|-----------------------------|---|------|
| Sensing amplitude [mV]      | ⌘ | 7.0  |
| Sensing polarity            |   | BIPL |
| Threshold [V]               | ⌘ | 0.6  |
| Pacing polarity             |   | BIPL |
| Pulse width [ms]            |   | 0.4  |
| Lead impedance [ $\Omega$ ] | ⌘ | 760  |
| Pacing polarity             |   | BIPL |

**Diagnostics**

|            |    |
|------------|----|
| Pacing [%] | 89 |
|------------|----|

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:51

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 21/34



**BIOTRONIK**  
excellence for life

| Follow-up | (1st interrog.) |
|-----------|-----------------|
|-----------|-----------------|

| Alerts and episodes |
|---------------------|
|---------------------|

|              |
|--------------|
| New episodes |
|--------------|

|                |
|----------------|
| 0 recording(s) |
|----------------|

**Test - Sensing****Test program**



| Mode             | R measurement VVI |
|------------------|-------------------|
| Basic rate [bpm] | 40                |
| Sensitivity [mV] | AUTO              |
| Sensing polarity | BIPL              |

**Measured values**

|                     |     |
|---------------------|-----|
| Mean rate [bpm]     | 54  |
| Min. amplitude [mV] | 5.7 |
| Mean amplitude [mV] | 6.2 |
| Max. amplitude [mV] | 7.4 |


**Freeze**

(R measurement VVI)

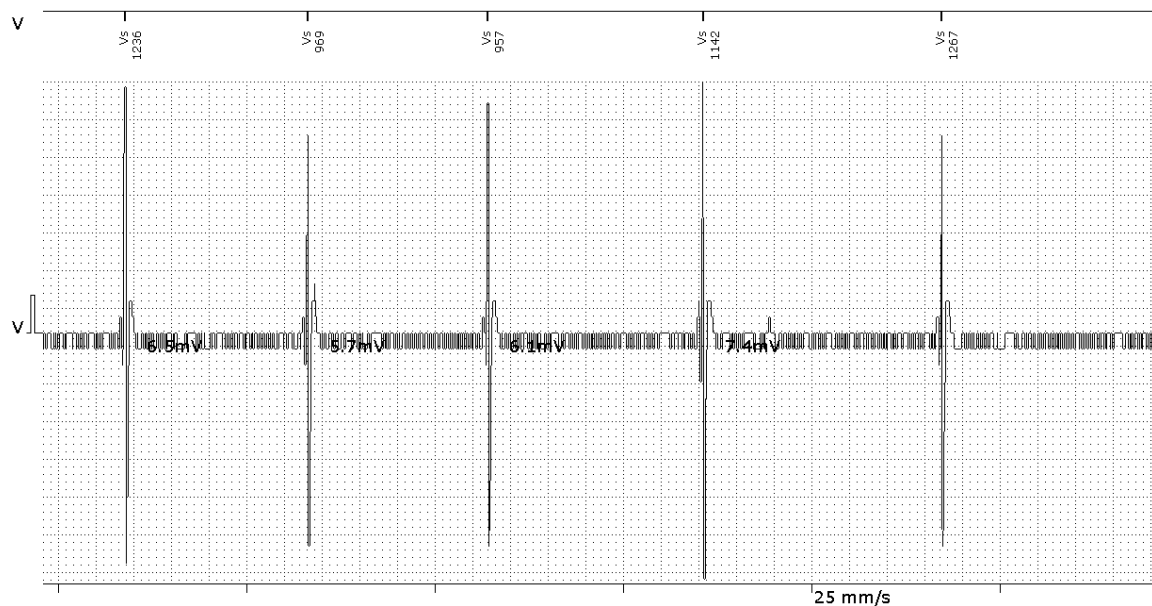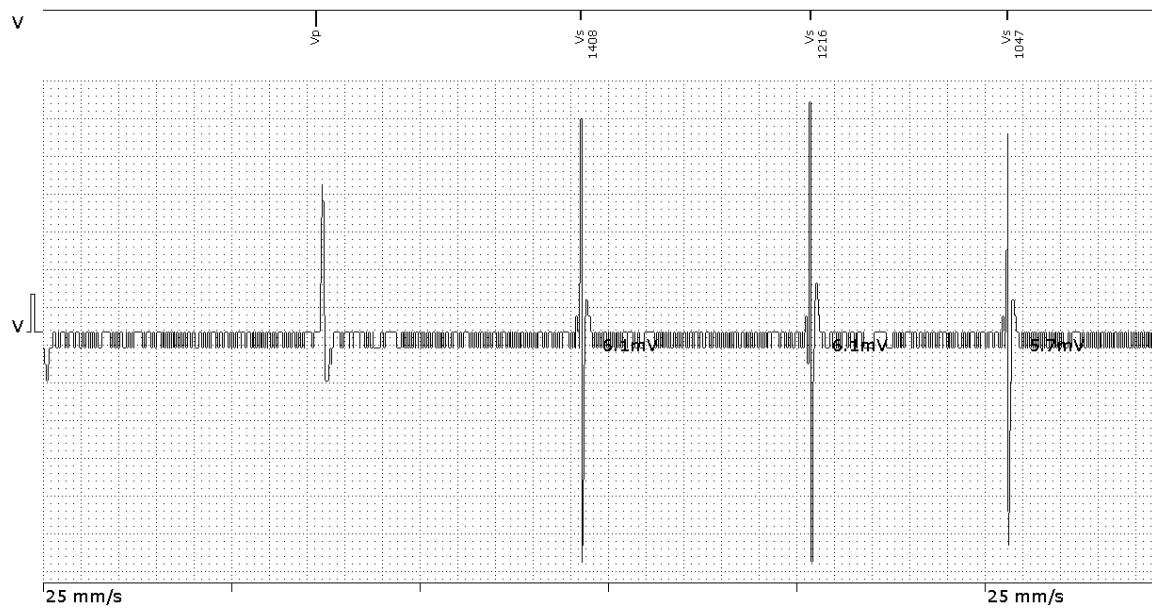

Freeze

(R measurement VVI)






Test - Pacing threshold

Test program

|                     |          |
|---------------------|----------|
| Mode                | Ven. VVI |
| Basic rate [bpm]    | 90       |
| Start amplitude [V] | 2.4      |
| Pulse width [ms]    | 0.4      |
| Pacing polarity     | BIPL     |
| Number of pulses    | 2        |

Selected value

|               |     |
|---------------|-----|
| Threshold [V] | 0.6 |
|---------------|-----|

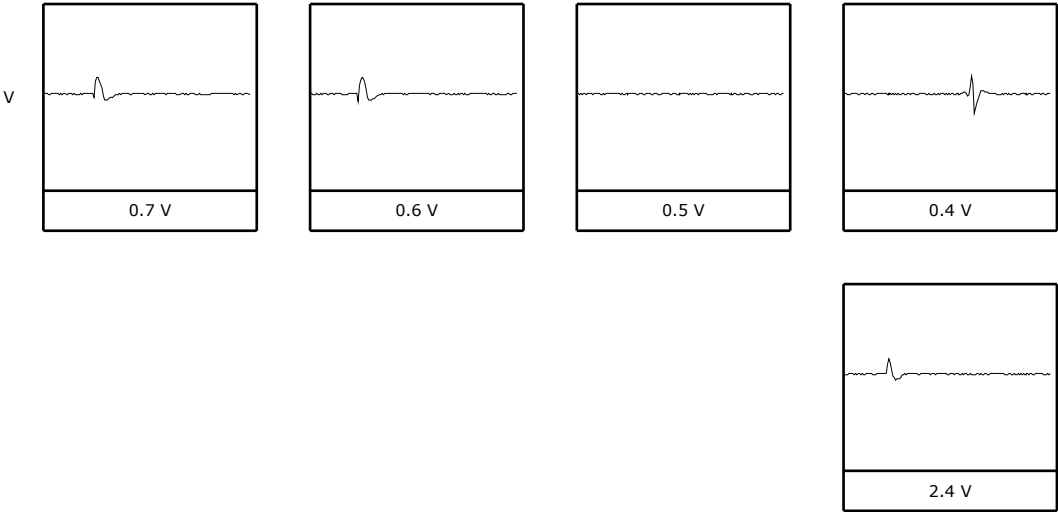

**Parameters - Overview**

|                             |   |             |
|-----------------------------|---|-------------|
| Mode                        |   | VVI-CLS     |
| Basic rate/Night rate [bpm] |   | 60/-----    |
| CLS                         |   | 120         |
| Sensor/Rate fading [bpm]    |   | 120/-----   |
| Upper rate response [bpm]   |   |             |
| Home Monitoring             |   | OFF         |
| Pulse amplitude [V]         | ⌵ | 2.4         |
| Pulse width [ms]            |   | 0.4         |
| Capture control             |   | ON          |
| Sensitivity [mV]            |   | AUTO        |
| Refract. period [ms]        |   | 250         |
| Sensing polarity            | ⌵ | BIPL        |
| Pacing polarity             | ⌵ | BIPL        |
| Calculated ERI              |   | 10 Y. 7 Mo. |

**Parameters - Bradycardia**

|                                |           |
|--------------------------------|-----------|
| Mode                           | VVI-CLS   |
| Basic rate/Night rate [bpm]    | 60/-----  |
| Basic rate [bpm]               | 60        |
| Night rate [bpm]               |           |
| Night begins                   |           |
| Night ends                     |           |
| Hysteresis [bpm]               |           |
| Repetitive/Scan cycles         |           |
| Magnet response                | ASync     |
| CLS                            | 120       |
| CLS response                   | Medium    |
| CLS resting rate control [bpm] | +20       |
| Vp required                    | No        |
| Sensor/Rate fading [bpm]       | 120/----- |
| Max. activity rate [bpm]       | 120       |
| Sensor gain                    | ⌀ AUTO    |
| Sensor threshold               | Medium    |
| Rate fading                    |           |
| Rate increase [bpm/cycle]      | 2         |
| Rate decrease [bpm/cycle]      | 0.5       |
| Upper rate response [bpm]      |           |

**Parameters - Bradycardia**

|                             |   |                 |
|-----------------------------|---|-----------------|
| Pulse amplitude [V]         | ⌘ | 2.4             |
| Pulse width [ms]            |   | 0.4             |
| Capture control             |   | ON              |
| Threshold test start [V]    |   | 2.4             |
| Safety margin [V]           |   | 1.0             |
| Search type                 |   | Time of day     |
| Interval [h]                |   |                 |
| Time of day                 |   | 00:30           |
| Status                      |   | OK              |
| Note                        |   | Search pending. |
| Last measured threshold [V] |   |                 |
| Date                        |   | XX/XX/XXXX      |
| Time                        |   | 00:00           |
| Sensitivity [mV]            |   | AUTO            |
| Refract. period [ms]        |   | 250             |
| Sensing polarity            | ⌘ | BIPL            |
| Pacing polarity             | ⌘ | BIPL            |
| Calculated ERI              |   | 10 Y. 7 Mo.     |

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:54

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023



**BIOTRONIK**

excellence for life

PSW 2301.A/1

Page 29/34

## Parameters - Home Monitoring

### General settings

|     |    |
|-----|----|
| PID | 89 |
|-----|----|

|                 |     |
|-----------------|-----|
| Home Monitoring | OFF |
|-----------------|-----|

|                              |  |
|------------------------------|--|
| Time of transmission [hh:mm] |  |
|------------------------------|--|

|           |  |
|-----------|--|
| High rate |  |
|-----------|--|

|                  |  |
|------------------|--|
| Event-based IEGM |  |
|------------------|--|

### Last message

|              |     |
|--------------|-----|
| Message type | --- |
|--------------|-----|

|                    |  |
|--------------------|--|
| Message created on |  |
|--------------------|--|

**Parameters - Diagnostics****Recording triggers**

|                           |          |
|---------------------------|----------|
| High rate                 | ON       |
| Patient trigger           | OFF      |
| Pre-trigger recording [%] | 75       |
| IEGM signal               | Filtered |

**Statistics**

|                              |       |
|------------------------------|-------|
| Start resting period [hh:mm] | 02:00 |
| Resting period duration [h]  | 4.0   |
| Thoracic impedance           | ON    |

**High rate**

|                            |     |
|----------------------------|-----|
| High rate limit [bpm]      | 150 |
| High rate counter [Events] | 8   |
| Enable lead check          | ON  |

| Parameters - Patient |            |                             |
|----------------------|------------|-----------------------------|
| ID                   |            |                             |
| Last name            | 295131-MRI |                             |
| First name           | Chen-Yan   |                             |
| Date of birth        | 04/25/1938 |                             |
| Gender               | Female     |                             |
| Date of implant      | 03/24/2023 |                             |
| Hospital, City       | CSMUH      |                             |
| Physician            | Dr.Su      |                             |
| Phone                |            |                             |
| Symptom              | B2<br>B3   | Dizzy spells<br>Bradycardia |
| ECG indication       |            |                             |
|                      | E6         | Atrial flutter/fib. + Brady |
| Etiology             |            |                             |
|                      |            | XXX                         |
| LVEF [%]             |            |                             |
|                      |            | XXX                         |
| NYHA                 |            |                             |
|                      |            | XXX                         |
| Remark               |            |                             |

Leads

| Lead model | Manufacturer | Serial number | Type | Implantation | Channels |
|------------|--------------|---------------|------|--------------|----------|
| Solia S 60 | Biotronik    | 8000717314    | BIPL | 03/24/2023   | RV       |
|            |              |               |      | XX/XX/XXXX   |          |
|            |              |               |      | XX/XX/XXXX   |          |
|            |              |               |      | XX/XX/XXXX   |          |

|                    |
|--------------------|
| Changed parameters |
|--------------------|

| Bradycardia                 |             |             |
|-----------------------------|-------------|-------------|
|                             | Previous    | Current     |
| Follow-up                   |             |             |
| Program count               | 3           | 4           |
| Capture control             |             |             |
| Capture control             | ATM         | ON          |
| Safety margin [V]           |             | 1.0         |
| Last measured threshold [V] | 0.6         |             |
| Date                        | 01/10/2024  | XX/XX/XXXX  |
| Time                        | 00:34       | 00:00       |
| Calculated ERI              |             |             |
| Calculated ERI              | 11 Y. 2 Mo. | 10 Y. 7 Mo. |



**Follow-up****Patient**

|                 |                      |
|-----------------|----------------------|
| Name            | 295131-MRI, Chen-Yan |
| Last follow-up  | 03/25/2023           |
| Date of implant | 03/24/2023           |

**Device status**

|                                |             |
|--------------------------------|-------------|
| Program count                  | 4           |
| Home Monitoring                | OFF         |
| MRI program                    | OFF         |
| Mode                           | VVI-CLS     |
| Basic rate [bpm]               | 60          |
| Pulse amplitude [V]            | ⌀ 2.4       |
| Pulse width [ms]               | 0.4         |
| Expected ERI                   | 10 Y. 7 Mo. |
| Battery status                 | OK          |
| Remaining battery capacity [%] | 95          |

**Test results**

|                             |       |
|-----------------------------|-------|
| Sensing amplitude [mV]      | 6.2   |
| Sensing polarity            | BIPL  |
| Threshold [V]               | 0.6   |
| Pacing polarity             | BIPL  |
| Pulse width [ms]            | 0.4   |
| Lead impedance [ $\Omega$ ] | ⌀ 760 |
| Pacing polarity             | BIPL  |

**Diagnostics**

|            |    |
|------------|----|
| Pacing [%] | 89 |
|------------|----|

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 01/10/2024 10:58

Last follow-up: 03/25/2023

Enitra 8 SR-T ( S/N: 70321996 PID: 89 )

Implantation: 03/24/2023

PSW 2301.A/1

Page 34/34

## Follow-up

### Alerts and episodes

New episodes

0 recording(s)