

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 1/25

Parameters - Overview		(1st interrog.)
Mode		VVI-CLS
Basic rate/Night rate [bpm]		60/-----
CLS		120
Sensor/Rate fading [bpm]		120/-----
Upper rate response [bpm]		
Home Monitoring		OFF
Pulse amplitude [V]	⚡	1.6
Pulse width [ms]		0.4
Capture control		ON
Sensitivity [mV]		AUTO
Refract. period [ms]		250
Sensing polarity	⚡	BIPL
Pacing polarity	⚡	BIPL
Calculated ERI		11 Y. 1 Mo.

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 2/25



BIOTRONIK

excellence for life

Parameters - Bradycardia		(1st interrog.)
Mode	VVI-CLS	
Basic rate/Night rate [bpm]	60/-----	
Basic rate [bpm]	60	
Night rate [bpm]		
Night begins		
Night ends		
Hysteresis [bpm]		
Repetitive/Scan cycles		
Magnet response	ASync	
CLS	120	
CLS response	Medium	
CLS resting rate control [bpm]	+20	
Vp required	No	
Sensor/Rate fading [bpm]	120/-----	
Max. activity rate [bpm]	120	
Sensor gain	⌀ AUTO	
Sensor threshold	Medium	
Rate fading		
Rate increase [bpm/cycle]	2	
Rate decrease [bpm/cycle]	0.5	
Upper rate response [bpm]		

Parameters - Bradycardia		(1st interrog.)
Pulse amplitude [V]	⌘	1.6
Pulse width [ms]		0.4
Capture control		ON
Threshold test start [V]		2.4
Safety margin [V]		1.0
Search type		Time of day
Interval [h]		
Time of day		00:30
Status		OK
Note		
Last measured threshold [V]		0.6
Date		09/13/2024
Time		00:34
Sensitivity [mV]		AUTO
Refract. period [ms]		250
Sensing polarity	⌘	BIPL
Pacing polarity	⌘	BIPL
Calculated ERI		11 Y. 1 Mo.

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 4/25

Parameters - Home Monitoring	(1st interrog.)
------------------------------	-----------------

General settings	
------------------	--

PID	89
-----	----

Home Monitoring	OFF
-----------------	-----

Time of transmission [hh:mm]	
------------------------------	--

High rate	
-----------	--

Event-based IEGM	
------------------	--

Last message	
--------------	--

Message type	---
--------------	-----

Message created on	
--------------------	--

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 5/25

Parameters - Diagnostics	(1st interrog.)
--------------------------	-----------------

Recording triggers	
--------------------	--

High rate	ON
Patient trigger	OFF
Pre-trigger recording [%]	75
IEGM signal	Filtered

Statistics	
------------	--

Start resting period [hh:mm]	02:00
Resting period duration [h]	4.0
Thoracic impedance	ON

High rate	
-----------	--

High rate limit [bpm]	150
High rate counter [Events]	8
Enable lead check	ON

295131-MRI, Chen-Yan

Date of birth: 04/25/1938
Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07
Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)
Implantation: 03/24/2023



Parameters - Patient		(1st interrog.)
ID		
Last name	295131-MRI	
First name	Chen-Yan	
Date of birth	04/25/1938	
Gender	Female	
Date of implant	03/24/2023	
Hospital, City	CSMUH	
Physician	Dr.Su	
Phone		
Symptom	B2 B3	Dizzy spells Bradycardia
ECG indication E6 Atrial flutter/fib. + Brady		
Etiology XXX		
LVEF [%] XXX		
NYHA XXX		
Remark		

Leads

Lead model	Manufacturer	Serial number	Type	Implantation	Channels
Solia S 60	Biotronik	8000717314	BIPL	03/24/2023	RV
				XX/XX/XXXX	
				XX/XX/XXXX	
				XX/XX/XXXX	

Diagnostics - Timing

(1st interrog.)

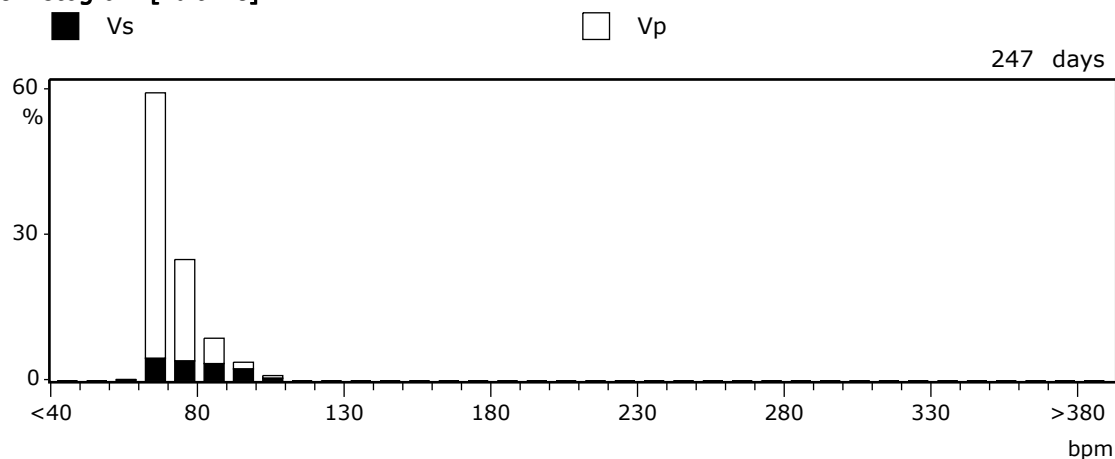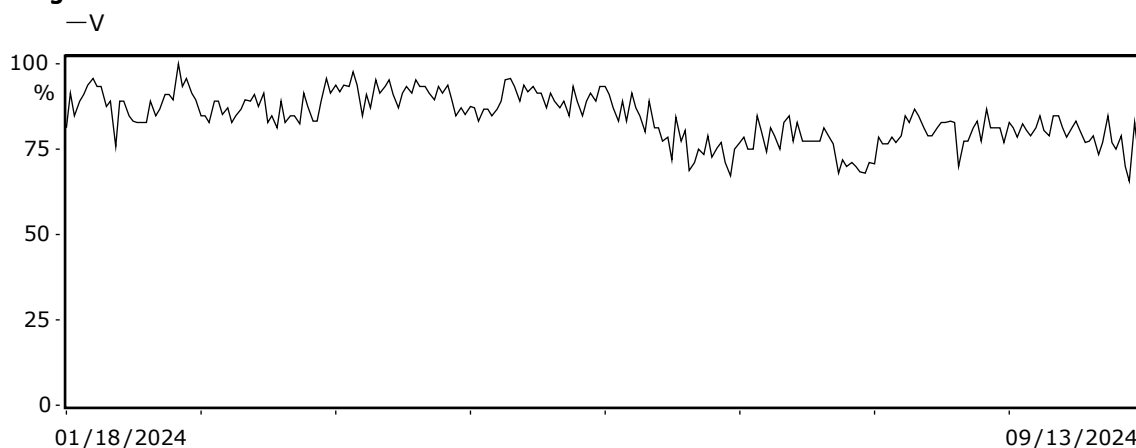Rate histogram [% time]**Event episodes and events****Pacing trend**

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023



BIOTRONIK

excellence for life

PSW 2302.A/1


Page 9/25

Diagnostics - 24 hours

(1st interrog.)


Rate

—V

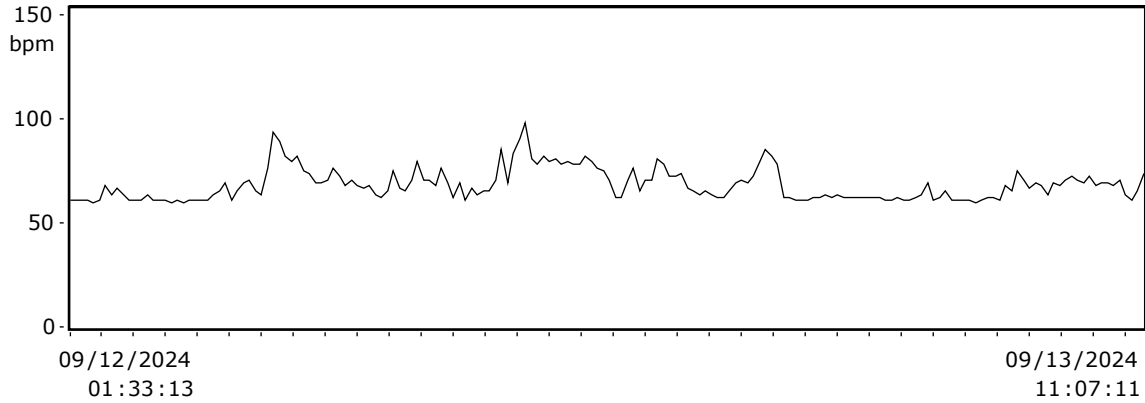

% paced

—V

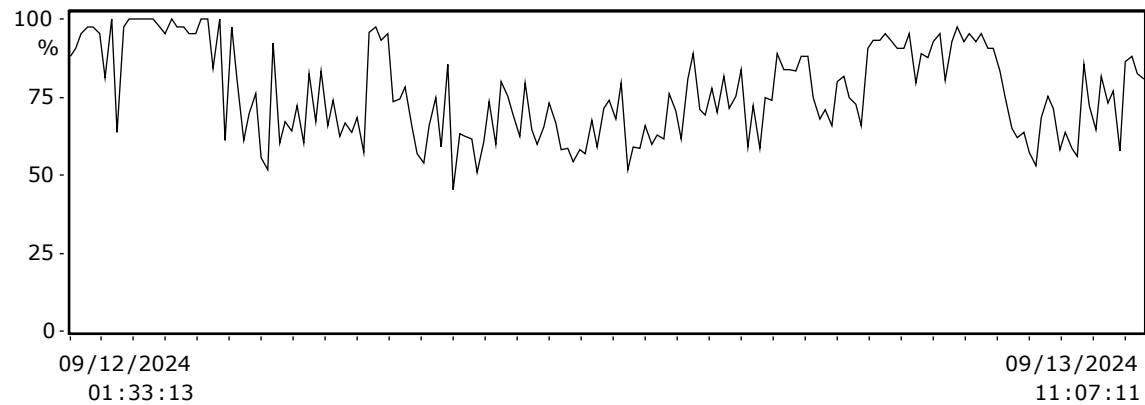


Start 01/10/2024

Diagnostics - More diag. - Event counters

(1st interrog.)

Event counters

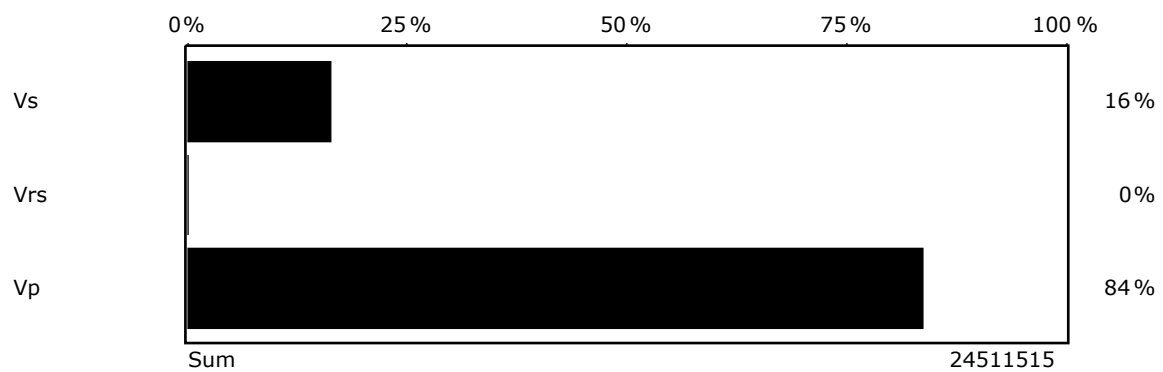


Start 01/10/2024

Diagnostics - More diag. - Pulse ampl. and threshold**(1st interrog.)**

Ventricle

✕ Threshold

◇ Amplitude

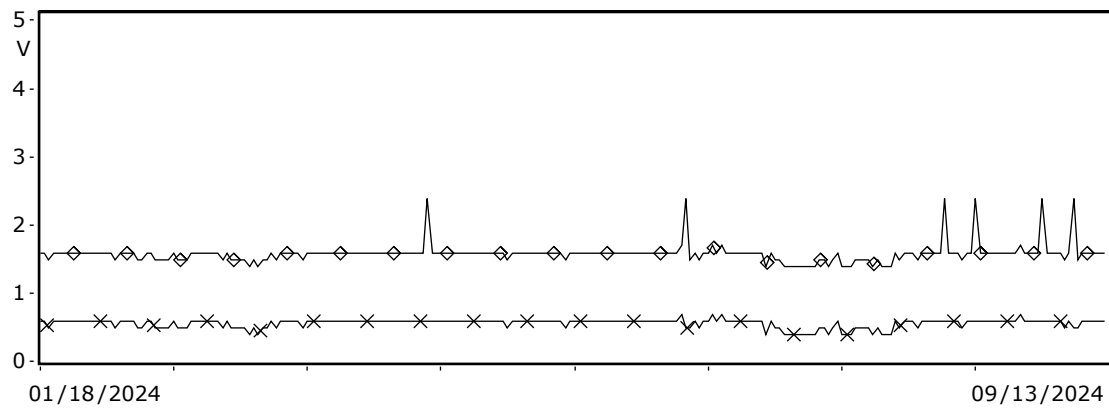

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023



BIOTRONIK

excellence for life


PSW 2302.A/1

Page 12/25

Diagnostics - More diag. - Sensor rate

(1st interrog.)

Sensor rate [% time]

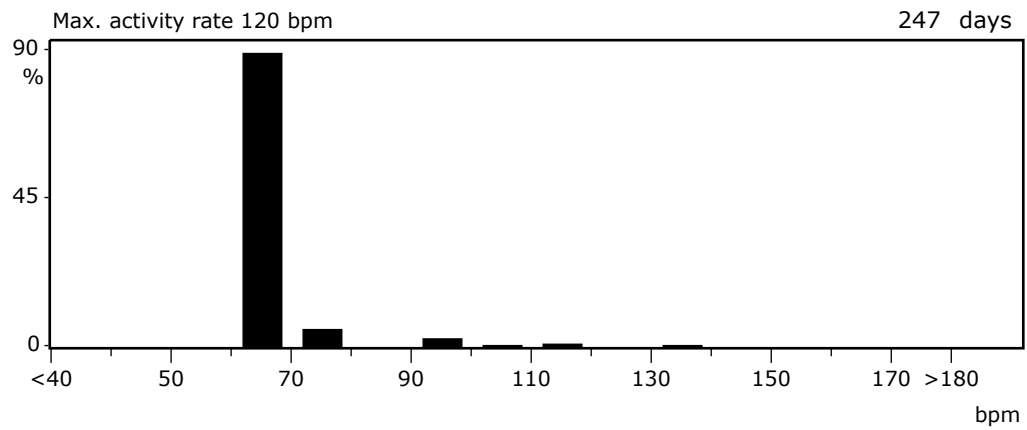

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 13/25



BIOTRONIK

excellence for life

Diagnostics - More diag. - Arrhythmia

(1st interrog.)

Ven. arrhythmia

High ventricular rate episodes [Count]

0

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023



BIOTRONIK

excellence for life

PSW 2302.A/1


Page 14/25

Diagnostics - More diag. - P/R wave trend

(1st interrog.)

P/R wave trend

—V

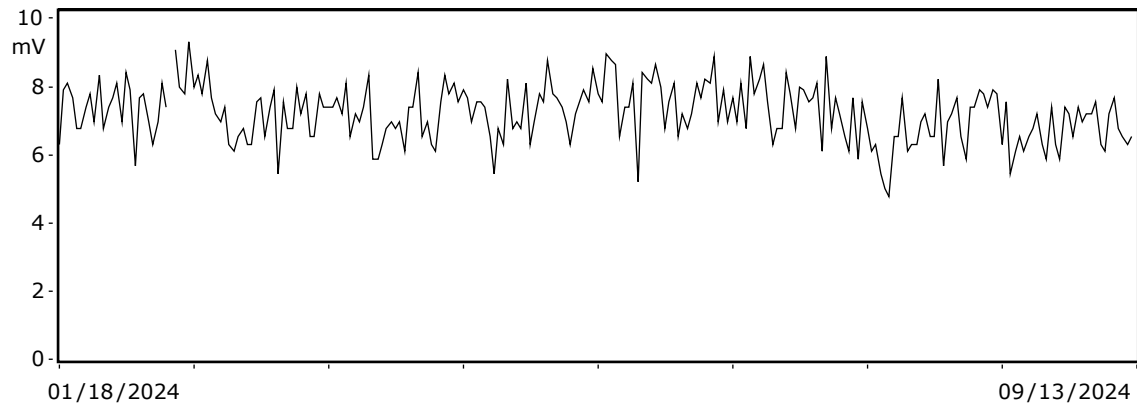

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023



BIOTRONIK

excellence for life

PSW 2302.A/1


Page 15/25

Diagnostics - More diag. - Lead impedance trend

(1st interrog.)

Lead impedance trend

—V

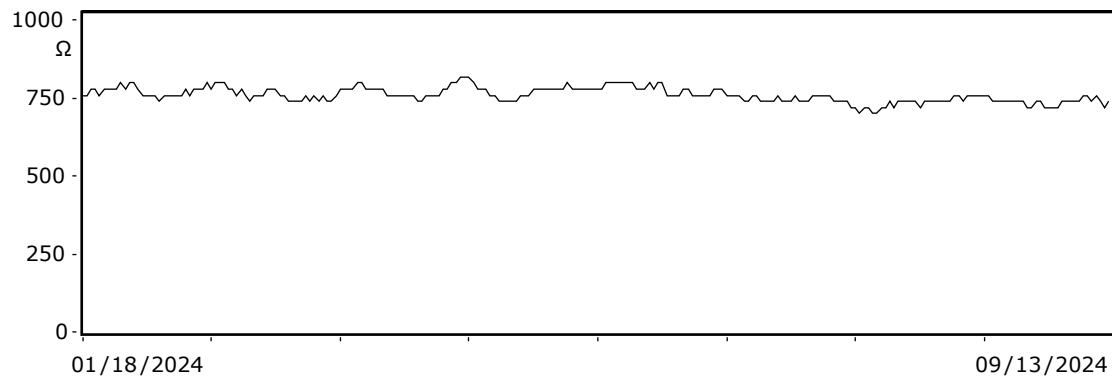


Start 01/10/2024

Follow-up - Details


(1st interrog.)

Rate histogram [% time]

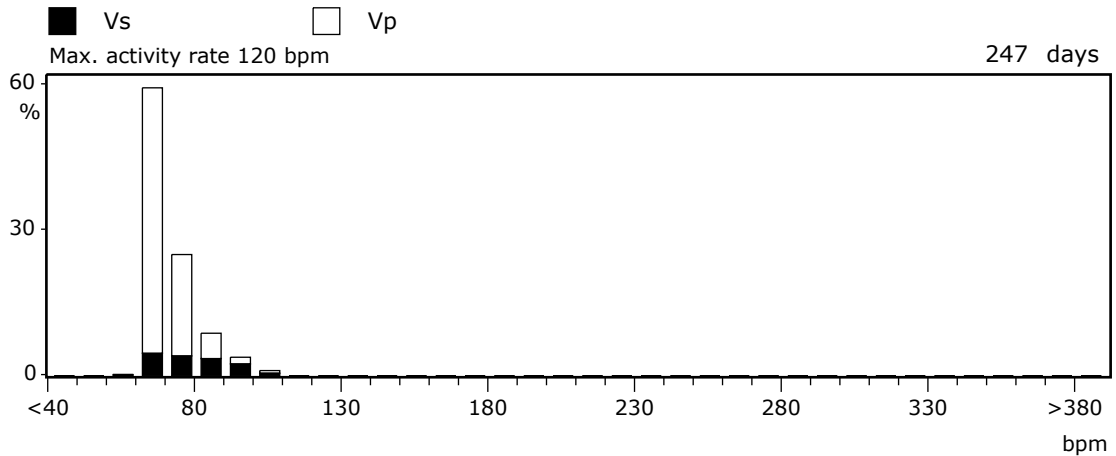


Long-term trends

Rate

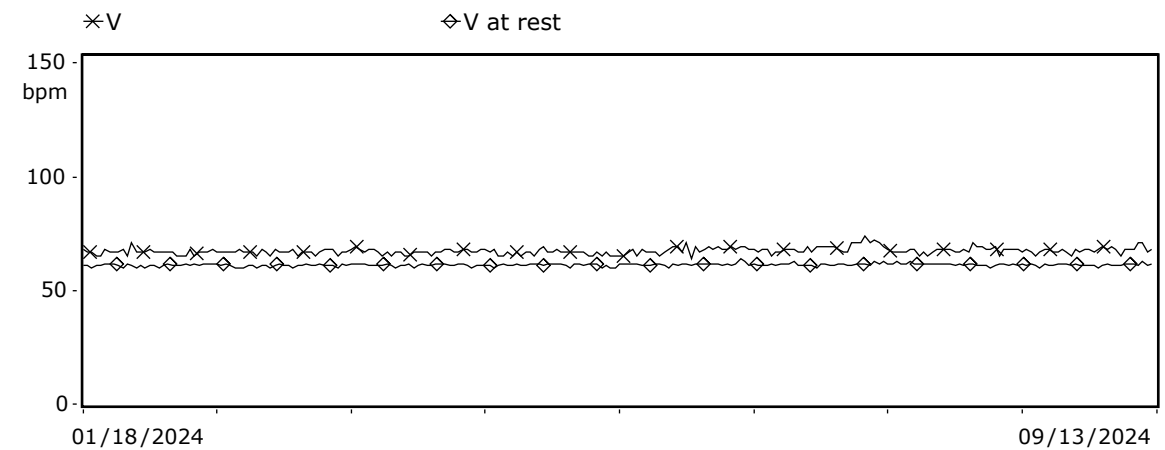

Patient activity

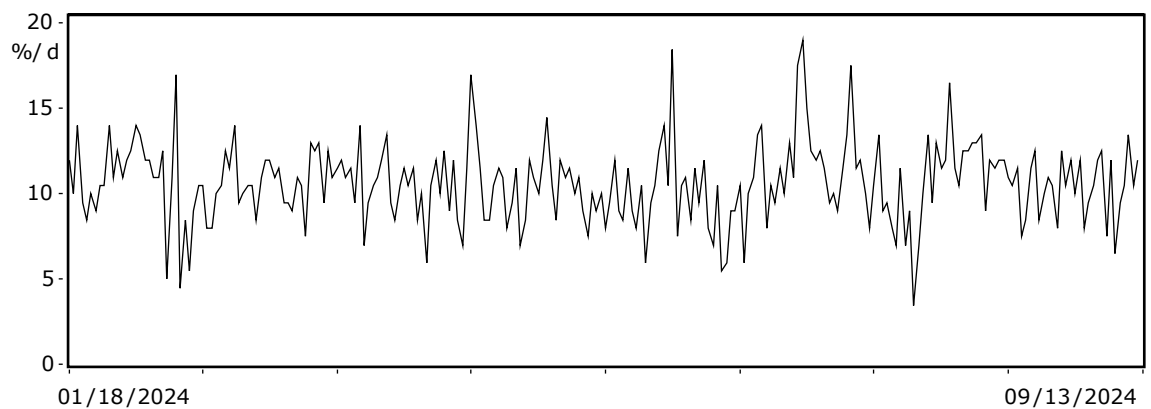


Start 01/10/2024

TrendView

(1st interrog.)


Mean rate

—V

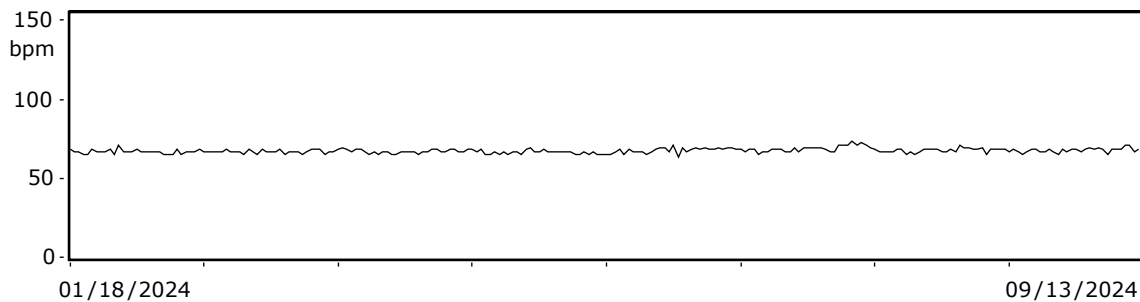


Pacing threshold

—V

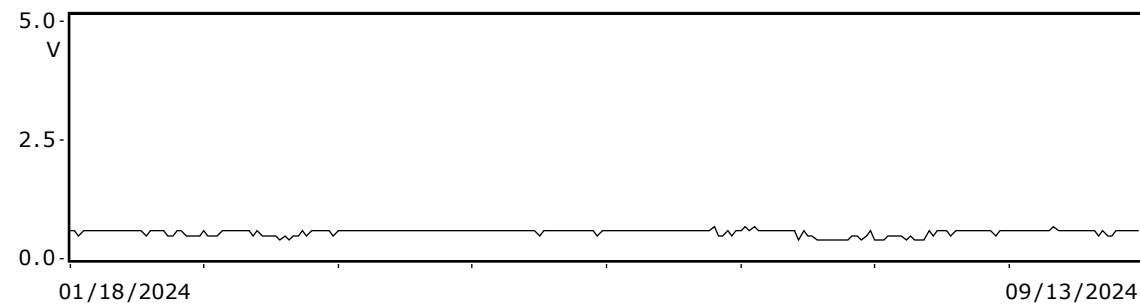


P/R wave amplitude

—V

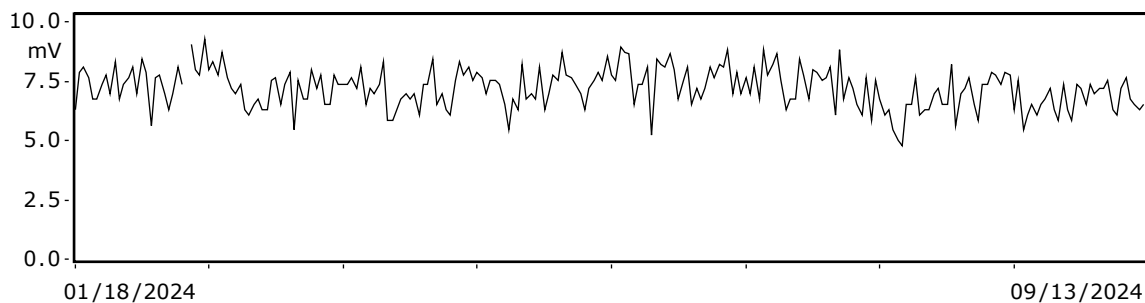

Lead impedance

—V

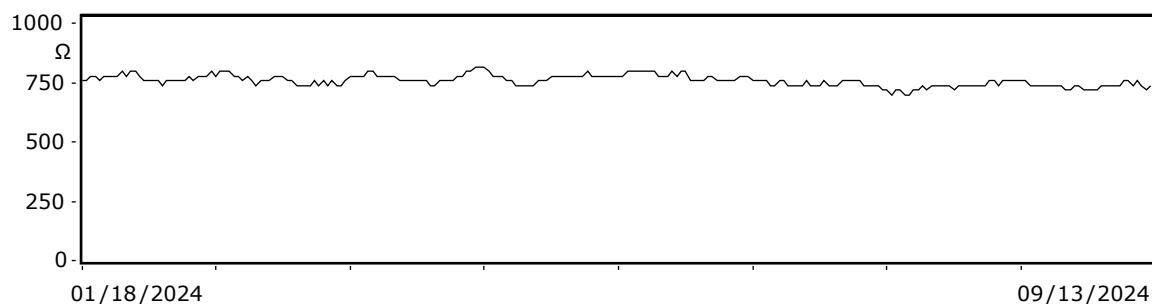

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 18/25



BIOTRONIK
excellence for life

TrendView

(1st interrog.)

Pacing in V [%]

84

Start 01/10/2024

295131-MRI, Chen-Yan

Date of birth: 04/25/1938
Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07
Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)
Implantation: 03/24/2023

Recordings - Episodes					
No.	Date	Duration	Trigger	MVR	PC

Follow-up	(1st interrog.)
-----------	-----------------

Patient

Name	295131-MRI, Chen-Yan
Last follow-up	01/10/2024
Date of implant	03/24/2023

Device status

Program count	4
Home Monitoring	OFF
MRI program	OFF

Mode	VVI-CLS
Basic rate [bpm]	60
Pulse amplitude [V]	1.6
Pulse width [ms]	0.4

Expected ERI	11 Y. 1 Mo.
Battery status	OK
Remaining battery capacity [%]	90

Test results

Sensing amplitude [mV]	5.0
Sensing polarity	BIPL

Threshold [V]	0.6
Pacing polarity	BIPL
Pulse width [ms]	0.4

Lead impedance [Ω]	702
Pacing polarity	BIPL

Diagnostics

Pacing [%]	84
------------	----

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:07

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 21/25



BIOTRONIK
excellence for life

Follow-up	(1st interrog.)
-----------	-----------------

Alerts and episodes

New episodes

0 recording(s)

**Test - Sensing****Test program**

Mode	R measurement VVI
Basic rate [bpm]	30
Sensitivity [mV]	AUTO
Sensing polarity	BIPL

Measured values

Mean rate [bpm]	63
Min. amplitude [mV]	5.2
Mean amplitude [mV]	5.8
Max. amplitude [mV]	6.1


Test - Pacing threshold

Test program

Mode	Ven. VVI
Basic rate [bpm]	90
Start amplitude [V]	1.6
Pulse width [ms]	0.4
Pacing polarity	BIPL
Number of pulses	3

Selected value

Threshold [V]	0.6
---------------	-----

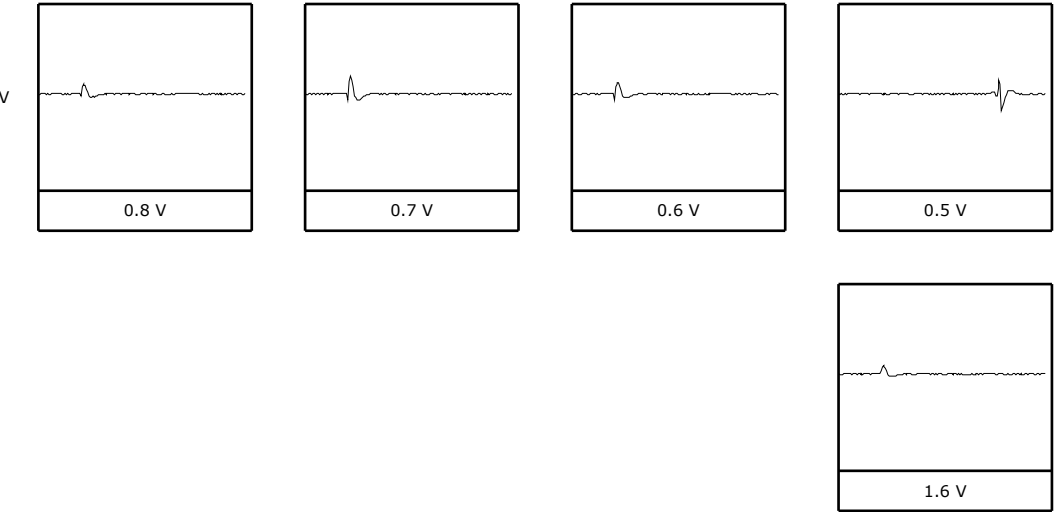

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:13

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

**BIOTRONIK**

excellence for life

PSW 2302.A/1

Page 24/25

Follow-up

Patient

Name	295131-MRI, Chen-Yan
Last follow-up	01/10/2024
Date of implant	03/24/2023

Device status

Program count	4
Home Monitoring	OFF
MRI program	OFF

Mode	VVI-CLS
Basic rate [bpm]	60
Pulse amplitude [V]	⌀ 1.6
Pulse width [ms]	0.4

Expected ERI	11 Y. 1 Mo.
Battery status	OK
Remaining battery capacity [%]	90

Test results

Sensing amplitude [mV]	⌀ 5.8
Sensing polarity	BIPL

Threshold [V]	0.6
Pacing polarity	BIPL
Pulse width [ms]	0.4

Lead impedance [Ω]	⌀ 702
Pacing polarity	BIPL

Diagnostics

Pacing [%]	84
------------	----

295131-MRI, Chen-Yan

Date of birth: 04/25/1938

Treating physician: Dr.Su

Recent follow-up: 09/13/2024 11:13

Last follow-up: 01/10/2024

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 25/25

Follow-up

Alerts and episodes

New episodes

0 recording(s)