
Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 1/10

Parameters - Overview		(1st interrog.)
Mode		VVI-CLS
Basic rate/Night rate [bpm]		60/-----
CLS		120
Sensor/Rate fading [bpm]		120/-----
Upper rate response [bpm]		
Home Monitoring		OFF
Pulse amplitude [V]	⚡	1.6
Pulse width [ms]		0.4
Capture control		ON
Sensitivity [mV]		AUTO
Refract. period [ms]		250
Sensing polarity	⚡	BIPL
Pacing polarity	⚡	BIPL
Calculated ERI		10 Y. 3 Mo.

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 2/10

Parameters - Bradycardia		(1st interrog.)
Mode		VVI-CLS
Basic rate/Night rate [bpm]		60/-----
Basic rate [bpm]		60
Night rate [bpm]		
Night begins		
Night ends		
Hysteresis [bpm]		
Repetitive/Scan cycles		
Magnet response		ASync
CLS		120
CLS response		Medium
CLS resting rate control [bpm]		+20
Vp required		No
Sensor/Rate fading [bpm]		120/-----
Max. activity rate [bpm]		120
Sensor gain	⌘	AUTO
Sensor threshold		Medium
Rate fading		
Rate increase [bpm/cycle]		2
Rate decrease [bpm/cycle]		0.5
Upper rate response [bpm]		

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 3/10



BIOTRONIK

excellence for life

Parameters - Bradycardia		(1st interrog.)
Pulse amplitude [V]	⌘	1.6
Pulse width [ms]		0.4
Capture control		ON
Threshold test start [V]		2.4
Safety margin [V]		1.0
Search type		Time of day
Interval [h]		
Time of day		00:30
Status		OK
Note		
Last measured threshold [V]		0.6
Date		09/12/2025
Time		00:34
Sensitivity [mV]		AUTO
Refract. period [ms]		250
Sensing polarity	⌘	BIPL
Pacing polarity	⌘	BIPL
Calculated ERI		10 Y. 3 Mo.

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 4/10

Parameters - Home Monitoring	(1st interrog.)
-------------------------------------	-----------------

General settings	
-------------------------	--

PID	89
Home Monitoring	OFF
Time of transmission [hh:mm]	
High rate	
Event-based IEGM	

Last message	
---------------------	--

Message type	---
Message created on	

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 5/10

Parameters - Diagnostics	(1st interrog.)
---------------------------------	-----------------

Recording triggers	
---------------------------	--

High rate	ON
Patient trigger	OFF
Pre-trigger recording [%]	75
IEGM signal	Filtered

Statistics	
-------------------	--

Start resting period [hh:mm]	02:00
Resting period duration [h]	4.0
Thoracic impedance	ON

High rate	
------------------	--

High rate limit [bpm]	150
High rate counter [Events]	8
Enable lead check	ON

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 6/10

Parameters - Patient	(1st interrog.)
----------------------	-----------------

ID

Last name	-----
-----------	-------

First name	-----
------------	-------

Date of birth	-----
---------------	-------

Gender	Female
--------	--------

Date of implant	03/24/2023
-----------------	------------

Hospital, City	CSMUH
----------------	-------

Physician	Dr.Su
-----------	-------

Phone	
-------	--

Symptom	B2 Dizzy spells
	B3 Bradycardia

ECG indication	E6 Atrial flutter/fib. + Brady
----------------	--------------------------------

Etiology	XXX
----------	-----

LVEF [%]	XXX
----------	-----

NYHA	XXX
------	-----

Remark	
--------	--

Leads

Lead model	Manufacturer	Serial number	Type	Implantation	Channels
Solia S 60	Biotronik	8000717314	BIPL	03/24/2023	RV
				XX/XX/XXXX	
				XX/XX/XXXX	
				XX/XX/XXXX	

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023


PSW 2302.A/1

Page 7/10

Diagnostics - Timing

(1st interrog.)


Rate histogram [% time]

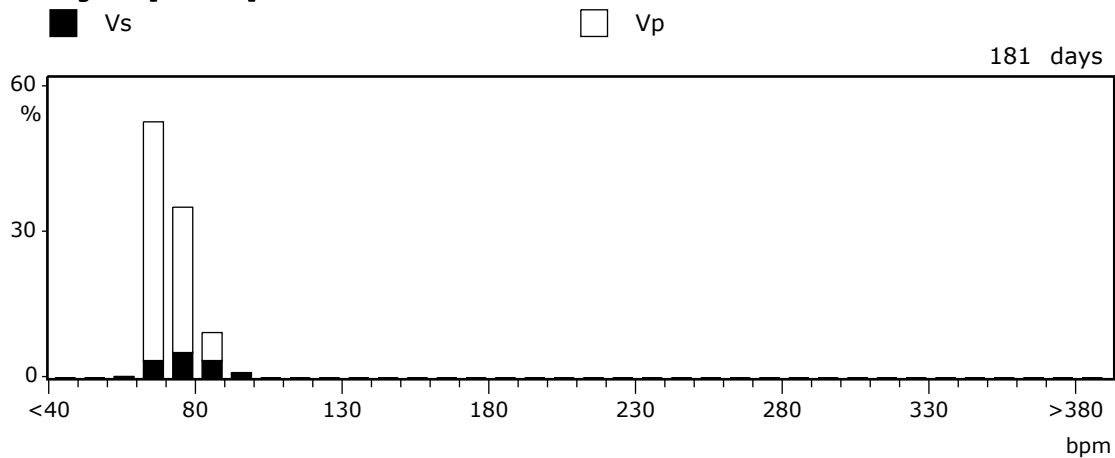

Event episodes and events



Pacing trend

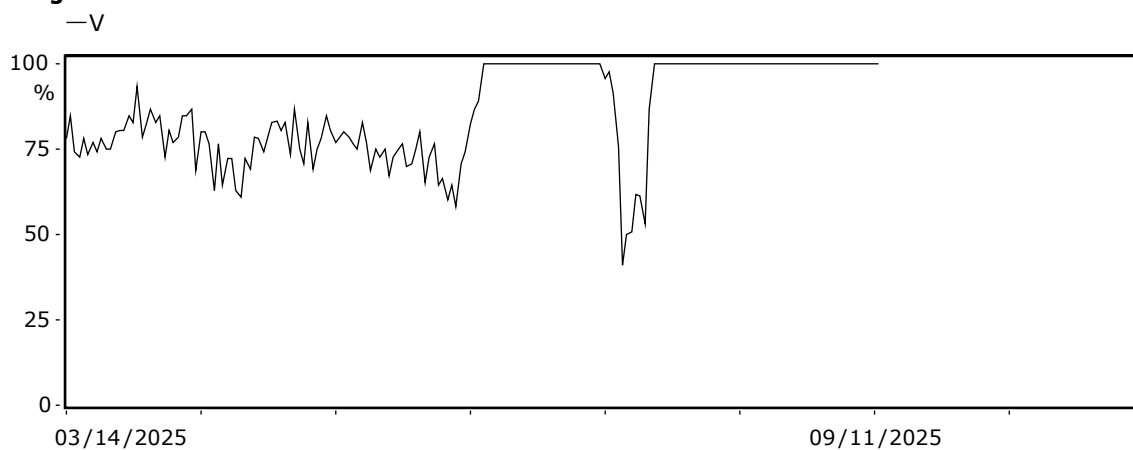

Start 03/14/2025

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023


PSW 2302.A/1

Page 8/10

Diagnostics - More diag. - Event counters

(1st interrog.)

Event counters

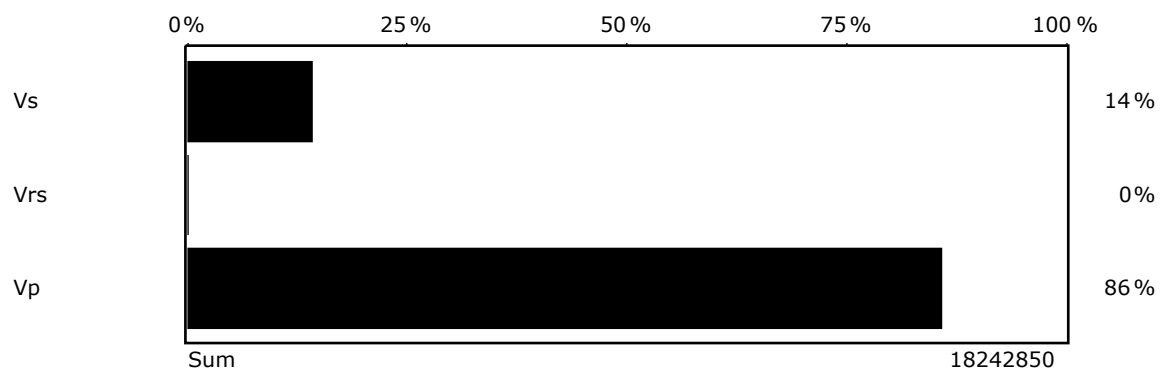

Start 03/14/2025

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023

PSW 2302.A/1

Page 9/10


Diagnostics - More diag. - Pulse ampl. and threshold

(1st interrog.)

Ventricle

✕ Threshold

◇ Amplitude

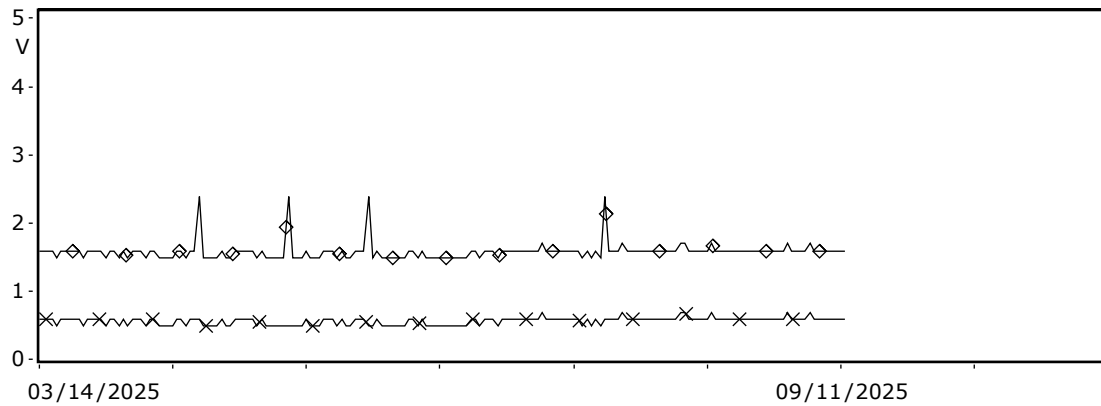

Start 03/14/2025

Date of birth: -----

Treating physician: Dr.Su

Recent follow-up: 09/12/2025 10:14

Last follow-up: 03/14/2025

Enitra 8 SR-T (S/N: 70321996 PID: 89)

Implantation: 03/24/2023


PSW 2302.A/1

Page 10/10

Diagnostics - More diag. - Sensor rate

(1st interrog.)

Sensor rate [% time]

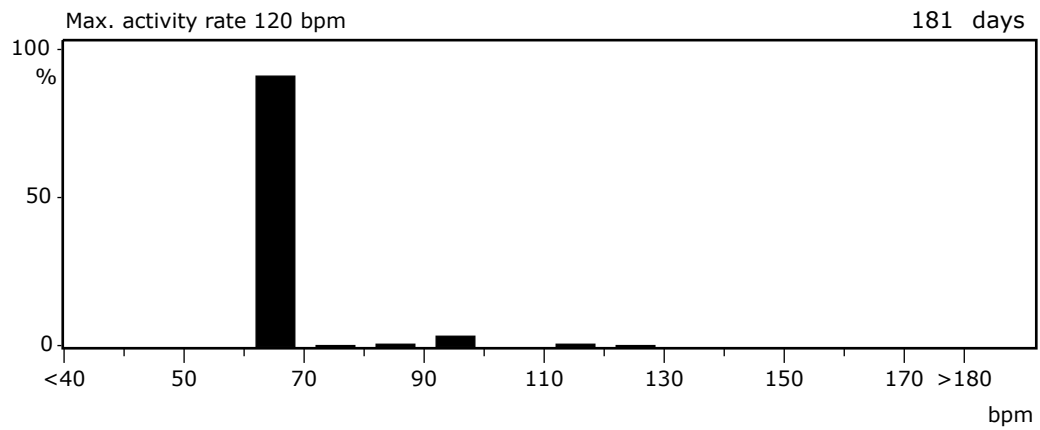

Start 03/14/2025