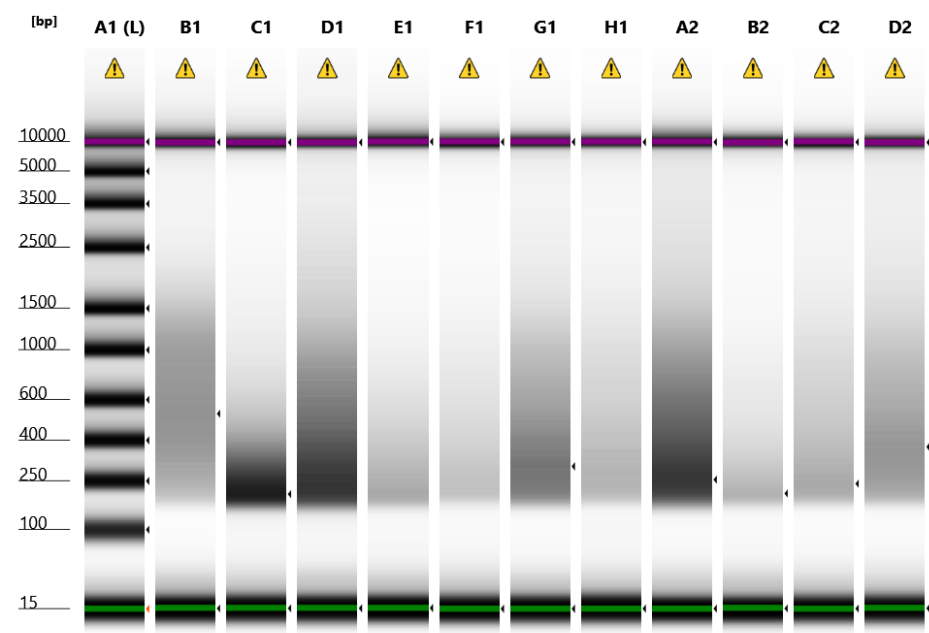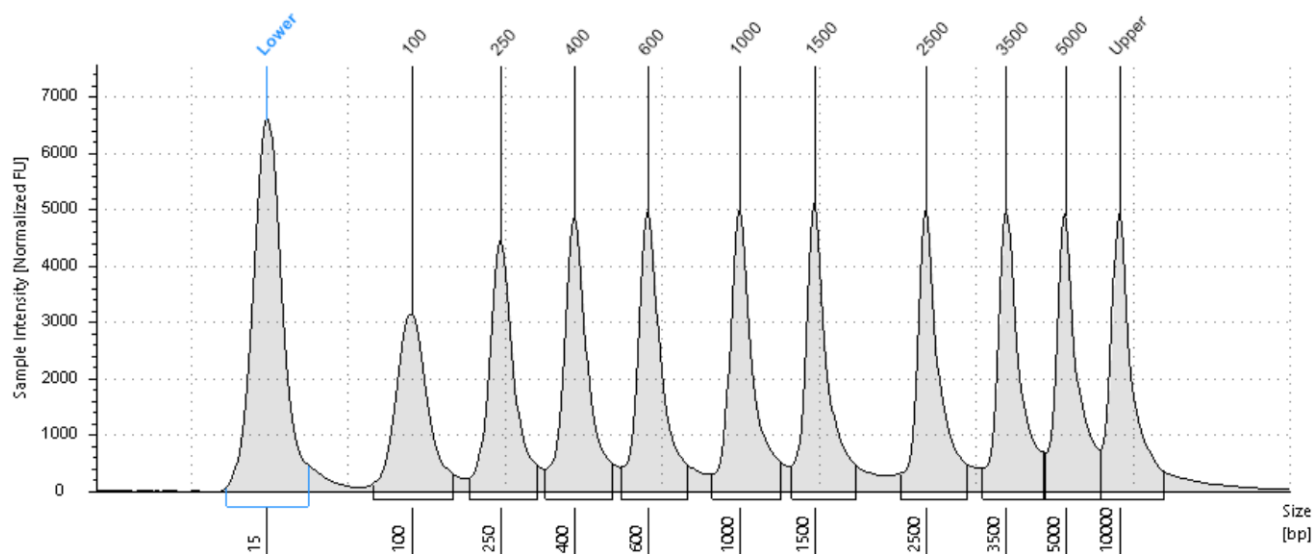# Filename: 2024-01-08 - 15.32.17.D5000

Default image (Contrast 100%)

Sample Info

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	44.2	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	1.67	2	⚠	Caution! Expired ScreenTape device
C1	10.5	3	⚠	Caution! Expired ScreenTape device
D1		4	⚠	Caution! Expired ScreenTape device
E1		5	⚠	Caution! Expired ScreenTape device
F1		6	⚠	Caution! Expired ScreenTape device
G1	5.64	7	⚠	Caution! Expired ScreenTape device
H1		8	⚠	Caution! Expired ScreenTape device
A2	12.7	9	⚠	Caution! Expired ScreenTape device
B2	2.33	10	⚠	Caution! Expired ScreenTape device
C2	3.26	11	⚠	Caution! Expired ScreenTape device
D2	4.47	12	⚠	Caution! Expired ScreenTape device

A1: Ladder

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A1	44.2	Ladder	⚠️	Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.75	-	795	-		Lower Marker
100	4.44	-	68.3	10.03		
250	4.97	-	30.6	11.24		
400	5.20	-	20.0	11.76		
600	5.19	-	13.3	11.72		
1000	5.16	-	7.94	11.67		
1500	5.02	-	5.15	11.34		
2500	4.84	-	2.98	10.93		
3500	4.76	-	2.09	10.76		
5000	4.67	-	1.44	10.55		
10000	3.25	3.25	0.500	-		Upper Marker

B1: 2
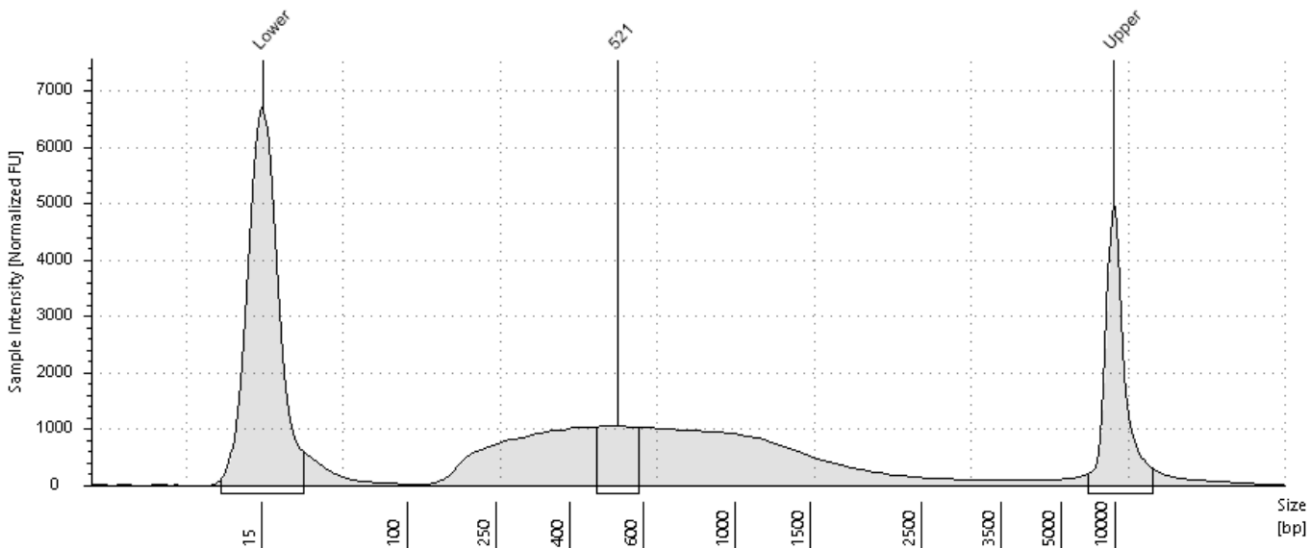
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
B1	1.67	2	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.59	-	779	-		Lower Marker
521	1.67	-	4.94	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C1: 3
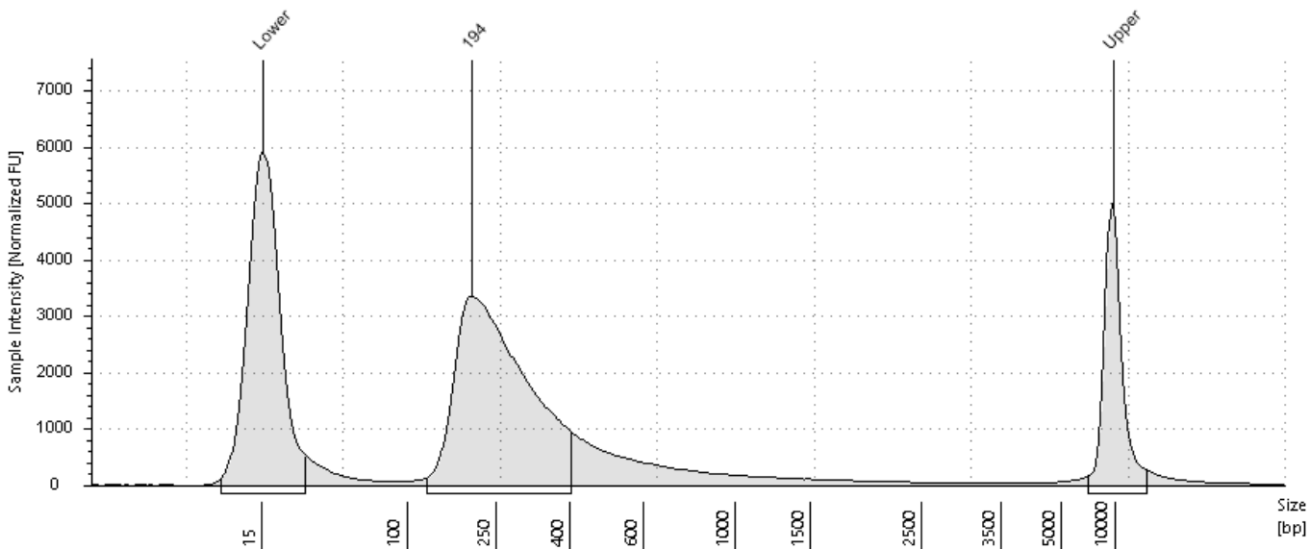
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C1	10.5	3	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.27	-	746	-		Lower Marker
194	10.5	-	82.9	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

D1: 4
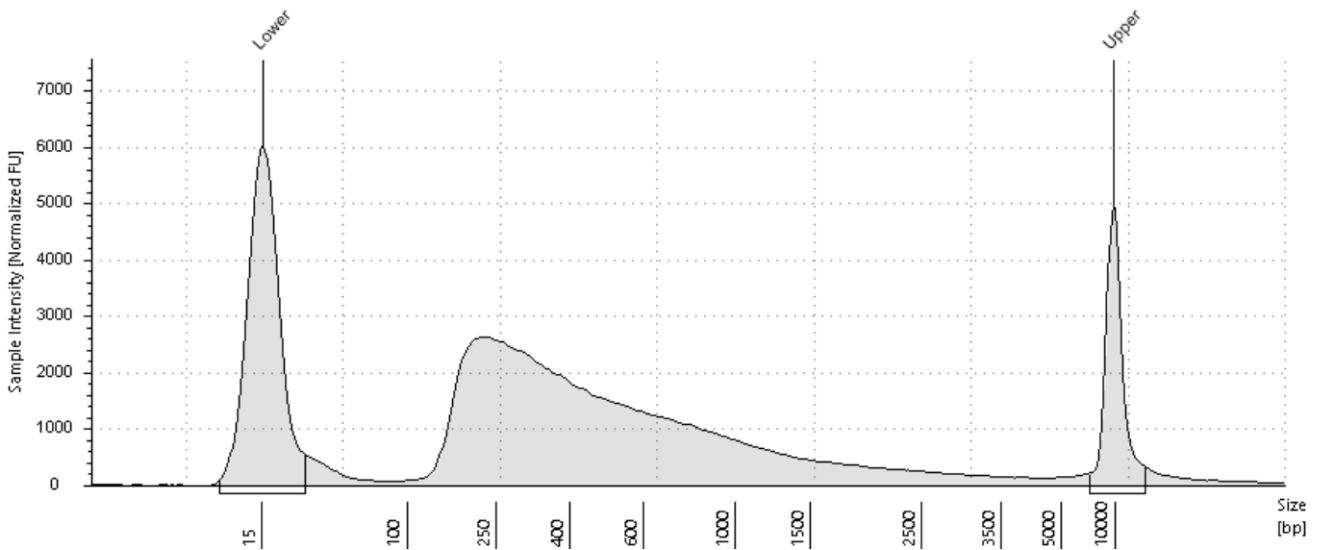
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D1		4	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.04	-	825	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

E1: 5
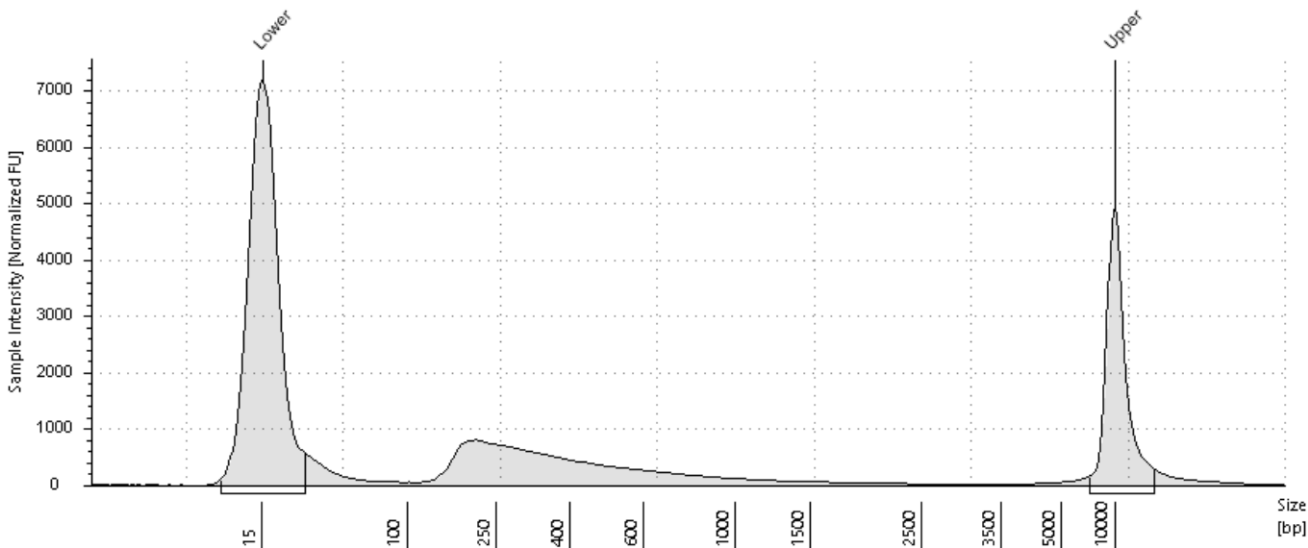
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
E1		5	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.88	-	808	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

F1: 6
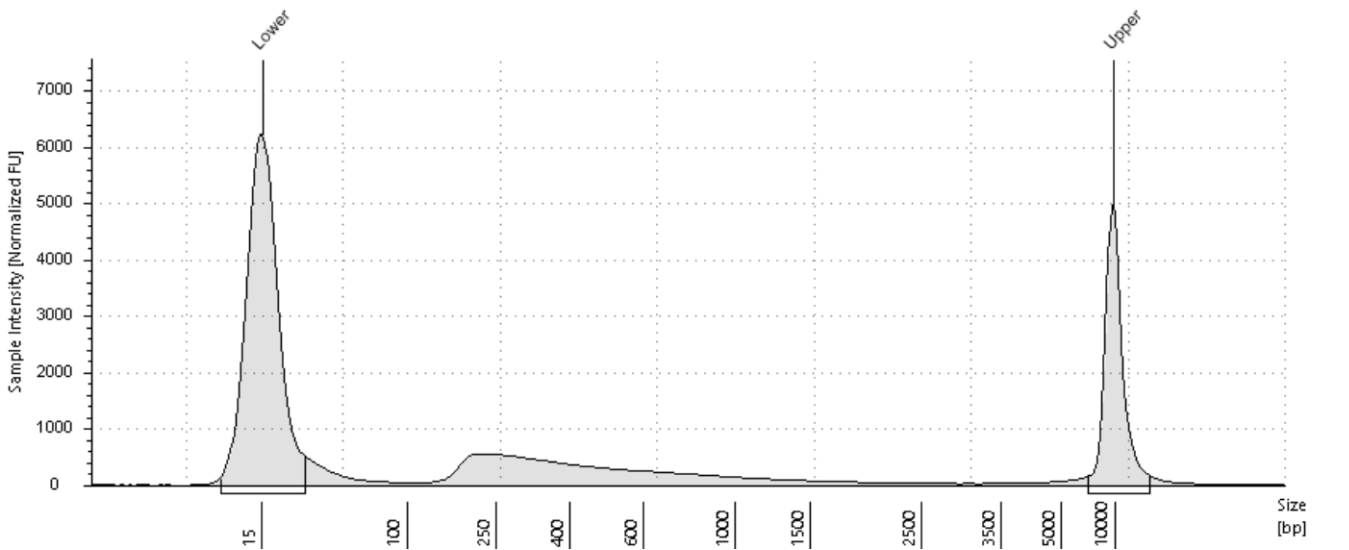
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
F1		6	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.45	-	764	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

G1: 7

Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
Gl	5.64	7	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.47	-	766	-		Lower Marker
296	5.64	-	29.3	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

H1: 8
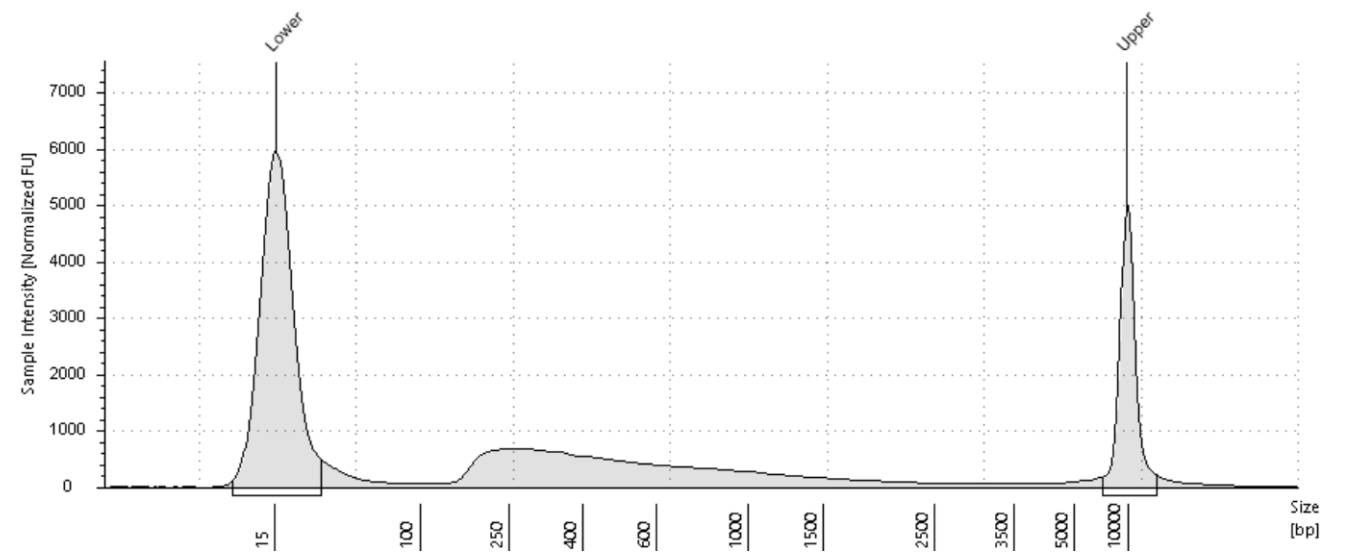
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
H1		8	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	8.40	-	862	-		Lower Marker
10000	3.25	3.25	0.500	-		Upper Marker

A2: 9
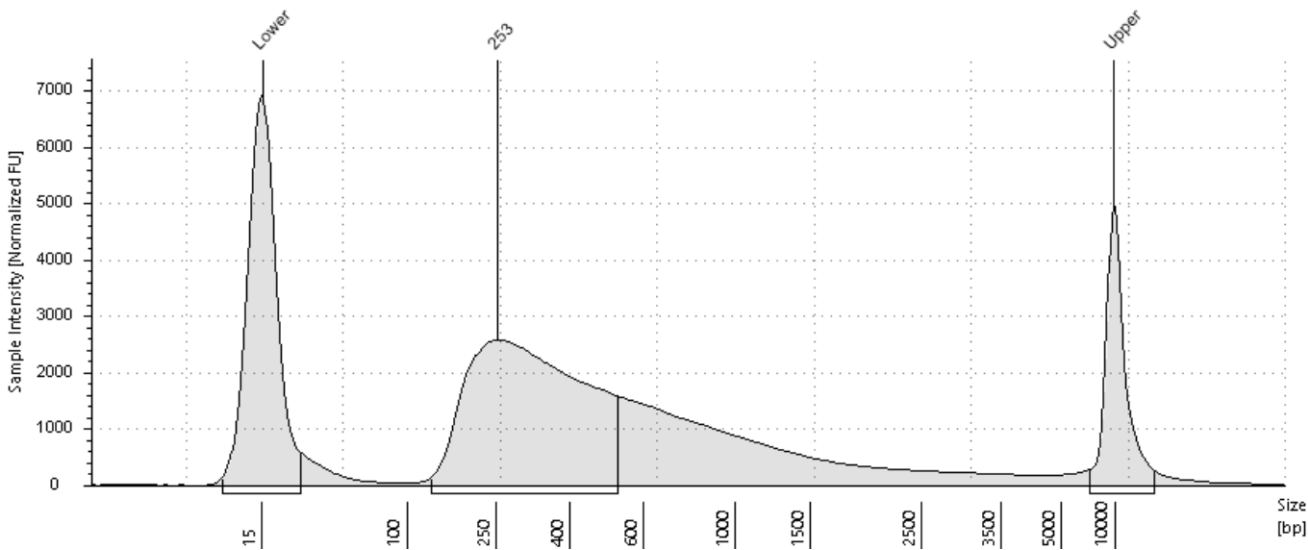
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
A2	12.7	9	⚠️	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.30	-	749	-		Lower Marker
253	12.7	-	77.4	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

B2: 10
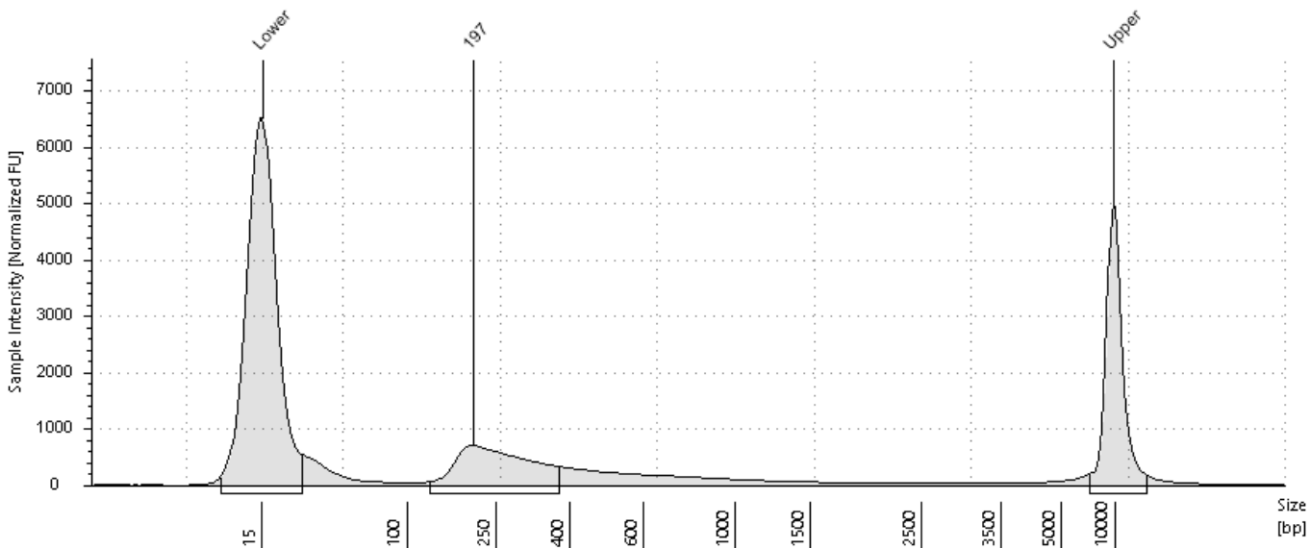
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
B2	2.33	10	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.79	-	799	-		Lower Marker
197	2.33	-	18.2	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

C2: 11
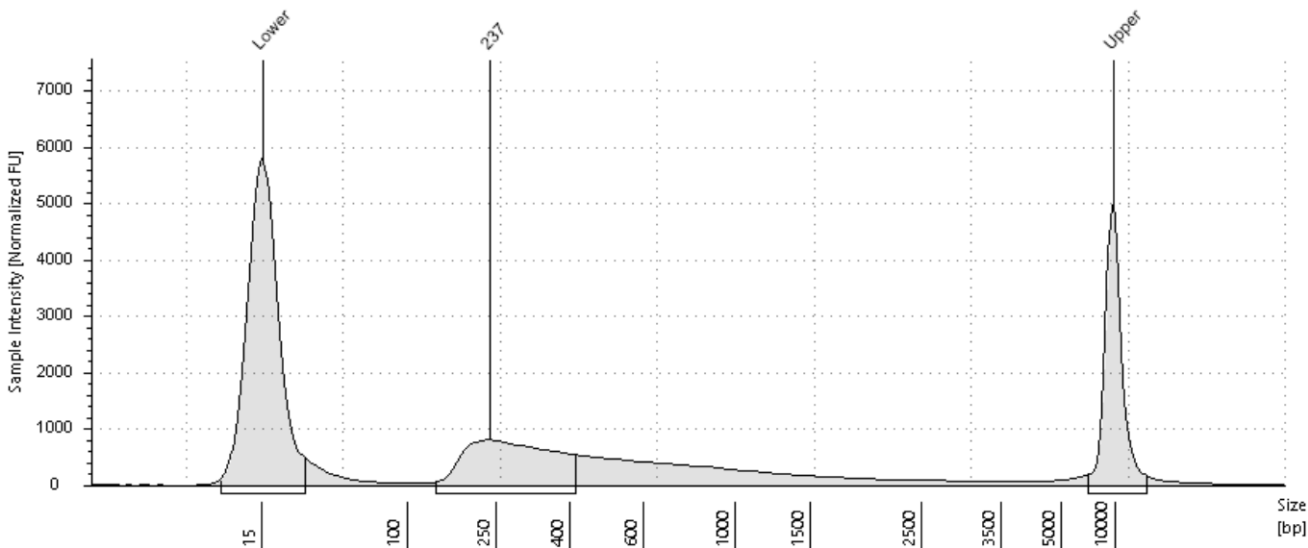
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
C2	3.26	11	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.12	-	730	-		Lower Marker
237	3.26	-	21.1	100.00		
10000	3.25	3.25	0.500	-		Upper Marker

D2: 12
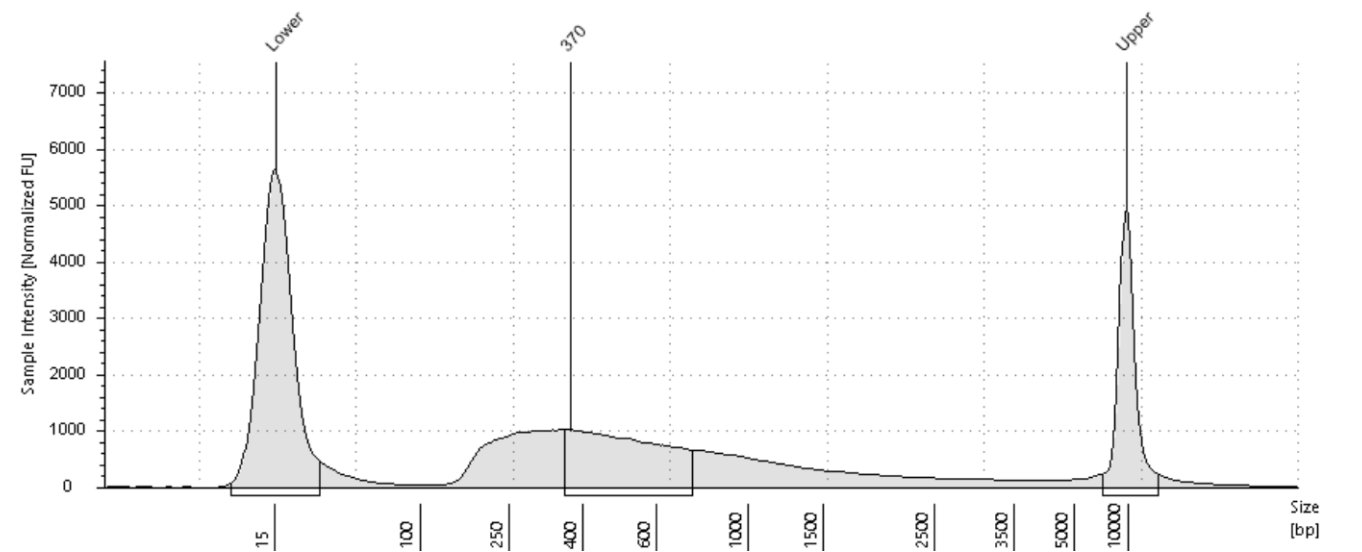
Sample Table

Well	Conc. [ng/µl]	Sample Description	Alert	Observations
D2	4.47	12	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/µl]	Assigned Conc. [ng/µl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
15	7.74	-	794	-		Lower Marker
370	4.47	-	18.6	100.00		
10000	3.25	3.25	0.500	-		Upper Marker