


Filename: 2022-06-30 - 14.09.24.D1000

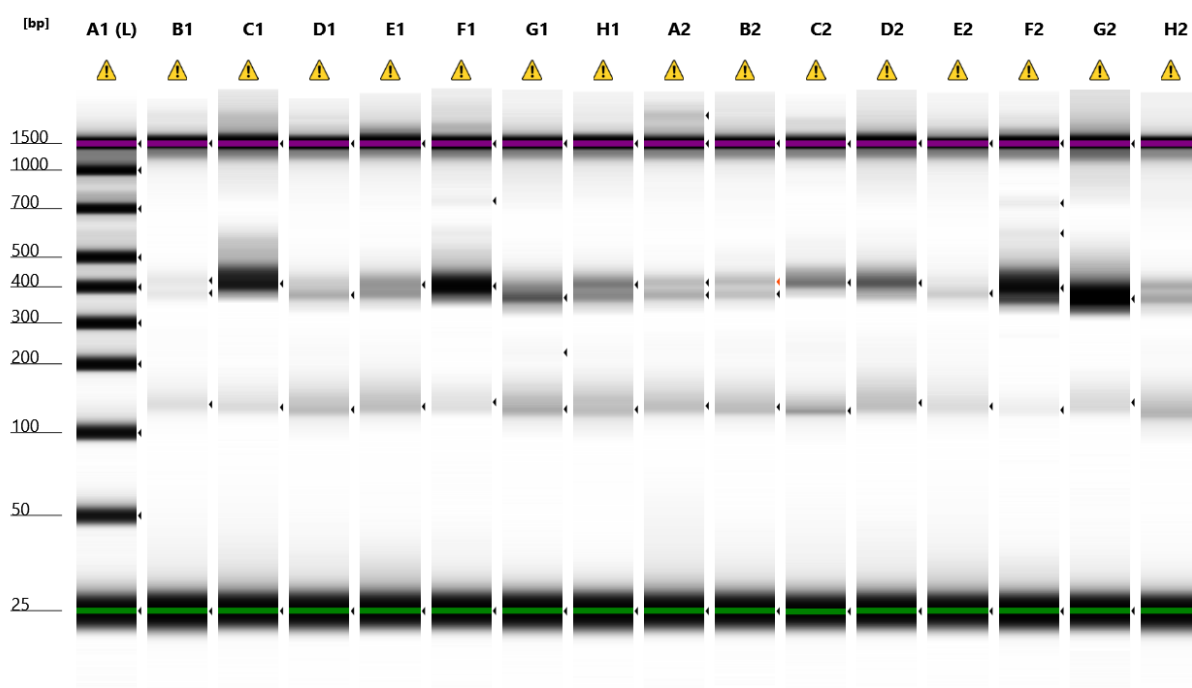

Default image (Contrast 132%)

Sample Info


Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	20.8	Ladder	⚠	Caution! Expired ScreenTape device; Ladder
B1	0.419	352	⚠	Caution! Expired ScreenTape device
C1	3.57	357	⚠	Caution! Expired ScreenTape device
D1	1.17	0HS3	⚠	Caution! Expired ScreenTape device
E1	1.12	9AZ5	⚠	Caution! Expired ScreenTape device
F1	4.60	9GT4	⚠	Caution! Expired ScreenTape device
G1	2.38	0DW46	⚠	Caution! Expired ScreenTape device
H1	1.06	2DW40	⚠	Caution! Expired ScreenTape device
A2	1.59	2EV3	⚠	Caution! Expired ScreenTape device; Peak out of Sizing Range
B2	1.20	2EV30	⚠	Caution! Expired ScreenTape device
C2	1.66	2EV34	⚠	Caution! Expired ScreenTape device
D2	2.12	2EV44	⚠	Caution! Expired ScreenTape device
E2	0.673	2IQ8	⚠	Caution! Expired ScreenTape device
F2	4.79	9GT46	⚠	Caution! Expired ScreenTape device
G2	7.49	4DW11	⚠	Caution! Expired ScreenTape device
H2	1.59	4EV14	⚠	Caution! Expired ScreenTape device

Compact Peak Table


Well	Sample Description	Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
A1	Ladder	25	6.71	-	413	-		Lower Marker
A1	Ladder	50	2.38	-	73.3	11.46		
A1	Ladder	100	2.56	-	39.3	12.29		
A1	Ladder	200	2.67	-	20.5	12.82		
A1	Ladder	300	2.69	-	13.8	12.93		
A1	Ladder	400	2.57	-	9.87	12.34		
A1	Ladder	500	2.69	-	8.27	12.93		
A1	Ladder	700	2.49	-	5.48	11.98		
A1	Ladder	1000	2.76	-	4.25	13.26		
A1	Ladder	1500	6.50	6.50	6.67	-		Upper Marker
B1	352	25	8.10	-	499	-		Lower Marker
B1	352	141	0.217	-	2.36	51.64		

BI	352	383	0.0877	-	0.352	20.90		
BI	352	422	0.115	-	0.420	27.46		
BI	352	1500	6.50	6.50	6.67	-		Upper Marker
CI	357	25	6.40	-	394	-		Lower Marker
CI	357	137	0.207	-	2.32	5.80		
CI	357	411	3.36	-	12.6	94.20		
CI	357	1500	6.50	6.50	6.67	-		Upper Marker
DI	0HS3	25	7.01	-	432	-		Lower Marker
DI	0HS3	134	0.557	-	6.39	47.62		
DI	0HS3	378	0.612	-	2.49	52.38		
DI	0HS3	1500	6.50	6.50	6.67	-		Upper Marker
EI	9AZ5	25	6.26	-	385	-		Lower Marker
EI	9AZ5	138	0.550	-	6.12	49.27		
EI	9AZ5	408	0.567	-	2.14	50.73		
EI	9AZ5	1500	6.50	6.50	6.67	-		Upper Marker
FI	9GT4	25	6.57	-	404	-		Lower Marker
FI	9GT4	145	0.116	-	1.23	2.52		
FI	9GT4	403	4.43	-	16.9	96.34		
FI	9GT4	762	0.0525	-	0.106	1.14		
FI	9GT4	1500	6.50	6.50	6.67	-		Upper Marker
GI	0DW46	25	7.22	-	444	-		Lower Marker
GI	0DW46	135	0.726	-	8.30	30.52		
GI	0DW46	228	0.0186	-	0.125	0.78		
GI	0DW46	370	1.63	-	6.79	68.70		
GI	0DW46	1500	6.50	6.50	6.67	-		Upper Marker
HI	2DW40	25	6.99	-	430	-		Lower Marker
HI	2DW40	134	0.301	-	3.46	28.34		
HI	2DW40	408	0.762	-	2.88	71.66		
HI	2DW40	1500	6.50	6.50	6.67	-		Upper Marker
A2	2EV3	25	7.17	-	441	-		Lower Marker
A2	2EV3	139	0.554	-	6.11	34.86		
A2	2EV3	378	0.382	-	1.56	24.04		
A2	2EV3	415	0.297	-	1.10	18.70		
A2	2EV3	1500	6.50	6.50	6.67	-		Upper Marker
A2	2EV3	2031	0.356	-	0.270	22.40		Peak outside of Sizing Range
B2	2EV30	25	7.24	-	446	-		Lower Marker
B2	2EV30	138	0.579	-	6.47	48.19		
B2	2EV30	380	0.290	-	1.17	24.11		
B2	2EV30	418	0.333	-	1.23	27.71		
B2	2EV30	1500	6.50	6.50	6.67	-		Upper Marker
C2	2EV34	25	6.85	-	421	-		Lower Marker
C2	2EV34	133	0.572	-	6.64	34.54		
C2	2EV34	416	1.08	-	4.01	65.46		
C2	2EV34	1500	6.50	6.50	6.67	-		Upper Marker
D2	2EV44	25	6.76	-	416	-		Lower Marker
D2	2EV44	144	0.592	-	6.33	27.86		
D2	2EV44	413	1.53	-	5.71	72.14		
D2	2EV44	1500	6.50	6.50	6.67	-		Upper Marker
E2	2IQ8	25	7.39	-	455	-		Lower Marker
E2	2IQ8	139	0.334	-	3.71	49.66		
E2	2IQ8	382	0.339	-	1.36	50.34		
E2	2IQ8	1500	6.50	6.50	6.67	-		Upper Marker
F2	9GT46	25	7.29	-	448	-		Lower Marker
F2	9GT46	133	0.0810	-	0.935	1.69		
F2	9GT46	397	4.56	-	17.7	95.21		
F2	9GT46	598	0.0871	-	0.224	1.82		
F2	9GT46	742	0.0611	-	0.127	1.28		
F2	9GT46	1500	6.50	6.50	6.67	-		Upper Marker
G2	4DW11	25	6.76	-	416	-		Lower Marker
G2	4DW11	144	0.284	-	3.03	3.79		
G2	4DW11	367	7.20	-	30.2	96.21		
G2	4DW11	1500	6.50	6.50	6.67	-		Upper Marker
H2	4EV14	25	7.47	-	460	-		Lower Marker
H2	4EV14	131	0.698	-	8.22	43.93		
H2	4EV14	365	0.508	-	2.14	31.99		
H2	4EV14	401	0.383	-	1.47	24.08		
H2	4EV14	1500	6.50	6.50	6.67	-		Upper Marker


A1: Ladder




B1: 352




C1: 357




D1: 0HS3




E1: 9AZ5




F1: 9GT4




G1: 0DW46




H1: 2DW40




A2: 2EV3




B2: 2EV30




C2: 2EV34




D2: 2EV44




E2: 2IQ8




F2: 9GT46




G2: 4DW11



H2: 4EV14




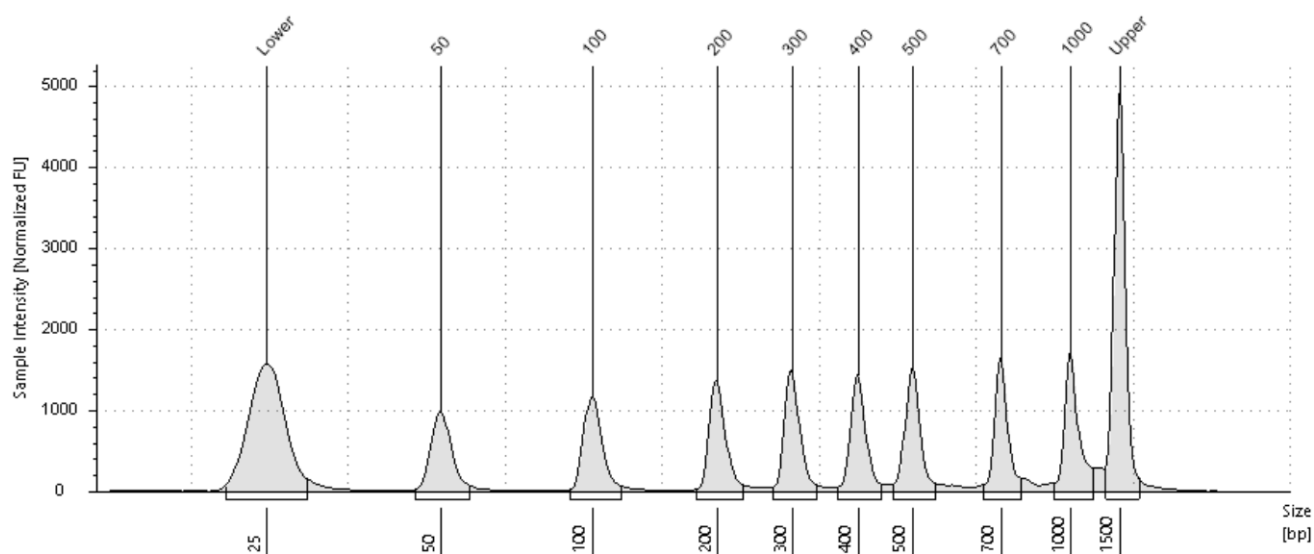A1: Ladder**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	20.8	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.71	-	413	-		Lower Marker
50	2.38	-	73.3	11.46		
100	2.56	-	39.3	12.29		
200	2.67	-	20.5	12.82		
300	2.69	-	13.8	12.93		
400	2.57	-	9.87	12.34		
500	2.69	-	8.27	12.93		
700	2.49	-	5.48	11.98		
1000	2.76	-	4.25	13.26		
1500	6.50	6.50	6.67	-		Upper Marker

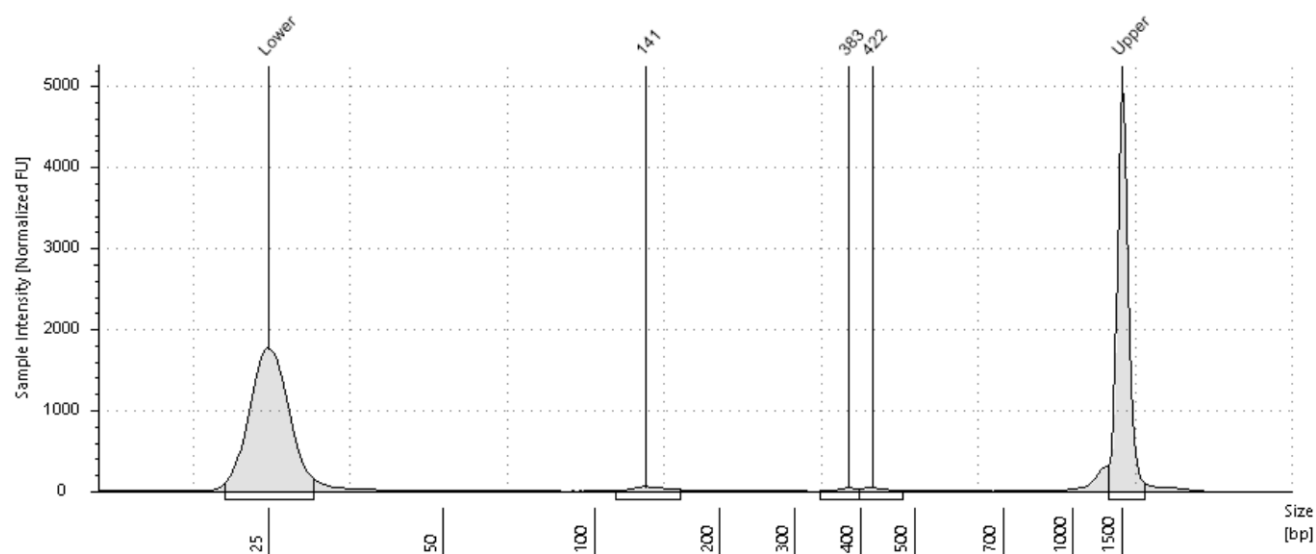
B1: 352**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B1	0.419	352	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	8.10	-	499	-		Lower Marker
141	0.217	-	2.36	51.64		
383	0.0877	-	0.352	20.90		
422	0.115	-	0.420	27.46		
1500	6.50	6.50	6.67	-		Upper Marker

C1: 357

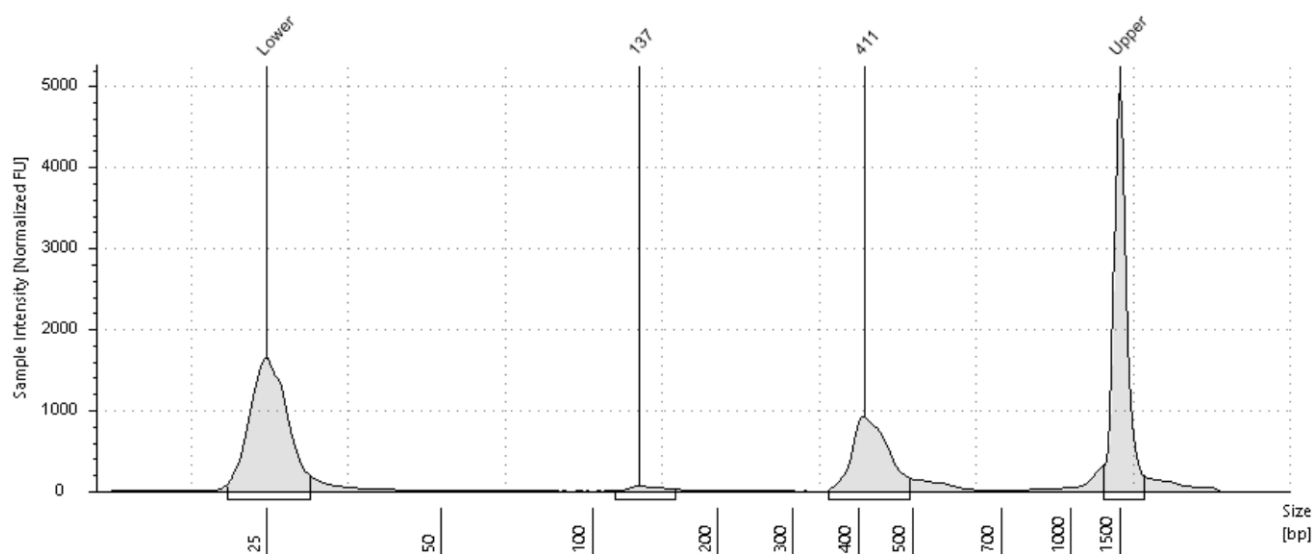


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C1	3.57	357	⚠	Caution! Expired ScreenTape device

Peak Table


Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.40	-	394	-		Lower Marker
137	0.207	-	2.32	5.80		
411	3.36	-	12.6	94.20		
1500	6.50	6.50	6.67	-		Upper Marker

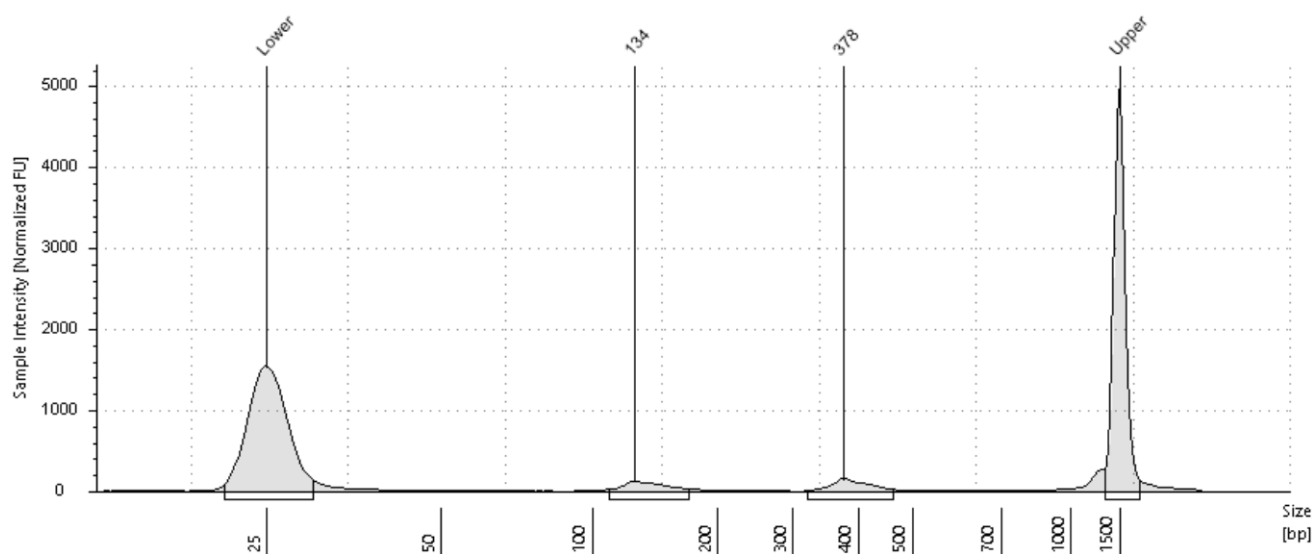D1: 0HS3**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
D1	1.17	0HS3	⚠	Caution! Expired ScreenTape device

Peak Table


Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.01	-	432	-		Lower Marker
134	0.557	-	6.39	47.62		
378	0.612	-	2.49	52.38		
1500	6.50	6.50	6.67	-		Upper Marker

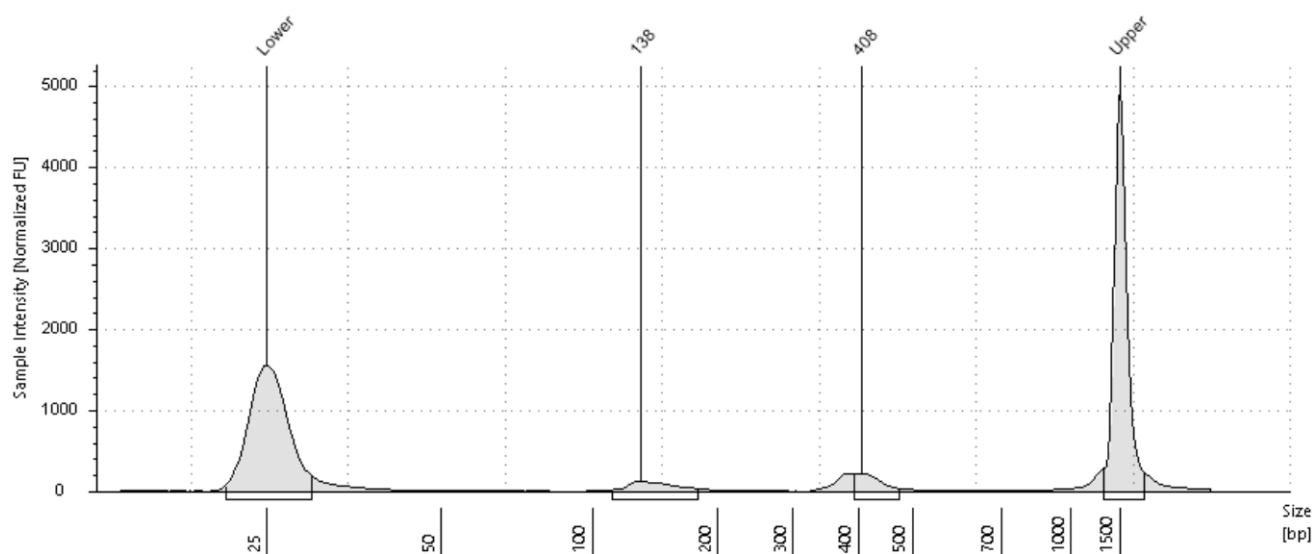E1: 9AZ5**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
E1	1.12	9AZ5	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.26	-	385	-		Lower Marker
138	0.550	-	6.12	49.27		
408	0.567	-	2.14	50.73		
1500	6.50	6.50	6.67	-		Upper Marker

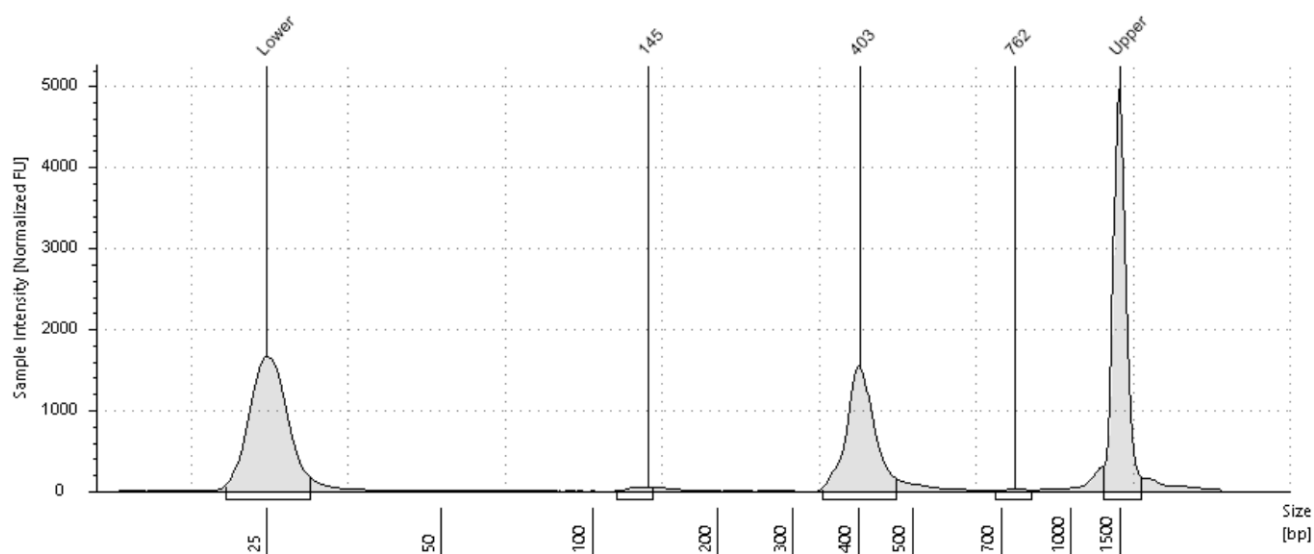
F1: 9GT4**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
F1	4.60	9GT4	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.57	-	404	-		Lower Marker
145	0.116	-	1.23	2.52		
403	4.43	-	16.9	96.34		
762	0.0525	-	0.106	1.14		
1500	6.50	6.50	6.67	-		Upper Marker

G1: 0DW46

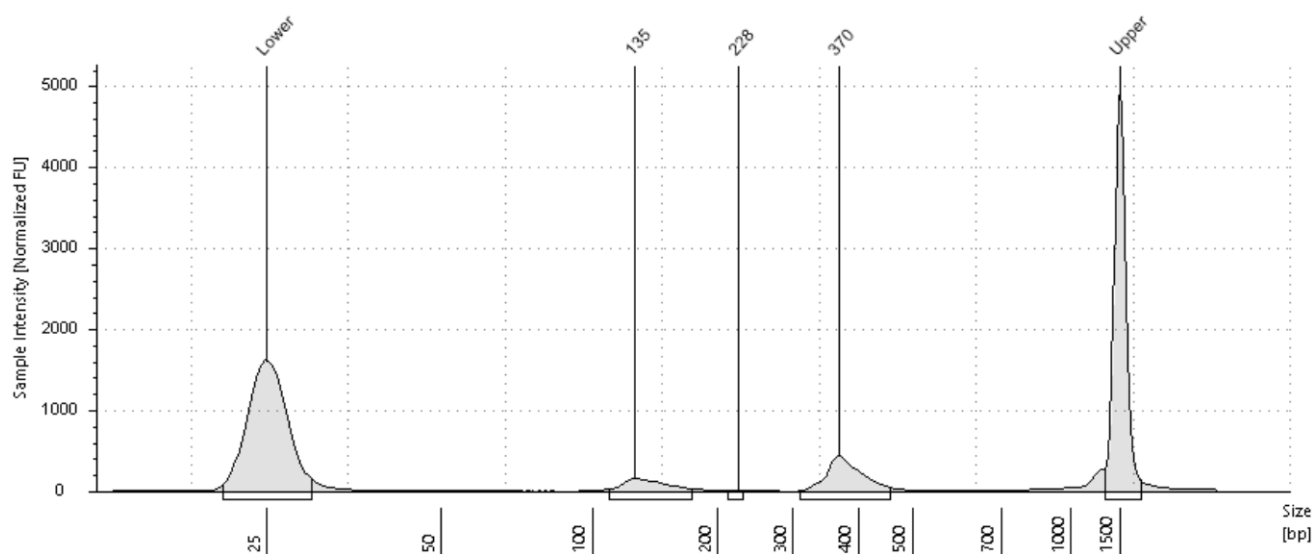


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
G1	2.38	0DW46	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.22	-	444	-		Lower Marker
135	0.726	-	8.30	30.52		
228	0.0186	-	0.125	0.78		
370	1.63	-	6.79	68.70		
1500	6.50	6.50	6.67	-		Upper Marker

H1: 2DW40

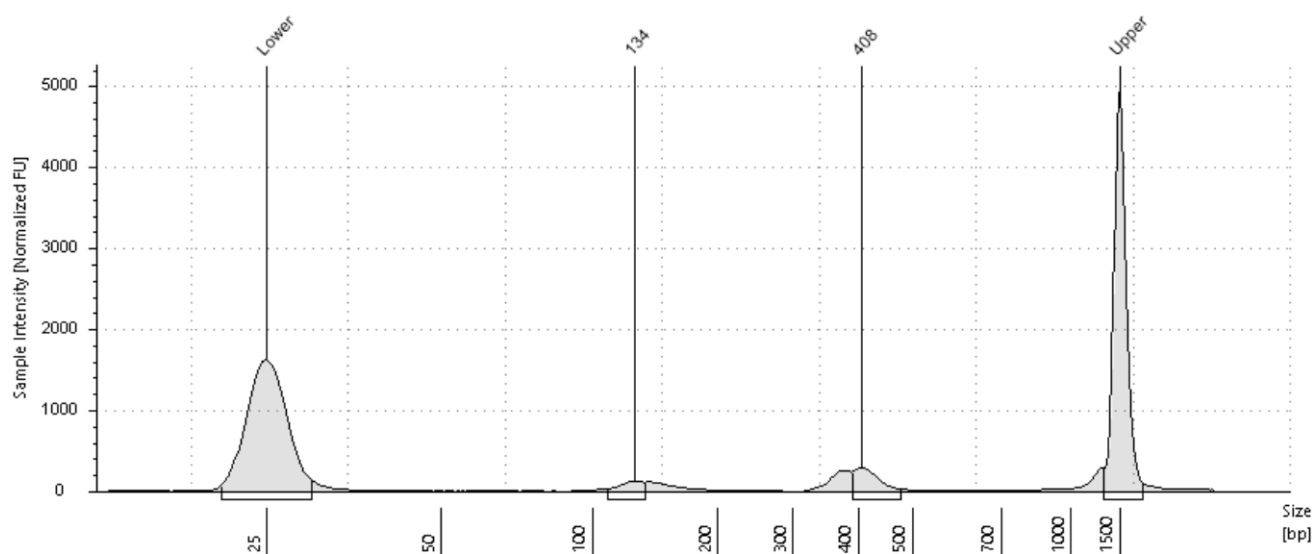


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
H1	1.06	2DW40	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.99	-	430	-		Lower Marker
134	0.301	-	3.46	28.34		
408	0.762	-	2.88	71.66		
1500	6.50	6.50	6.67	-		Upper Marker

A2: 2EV3

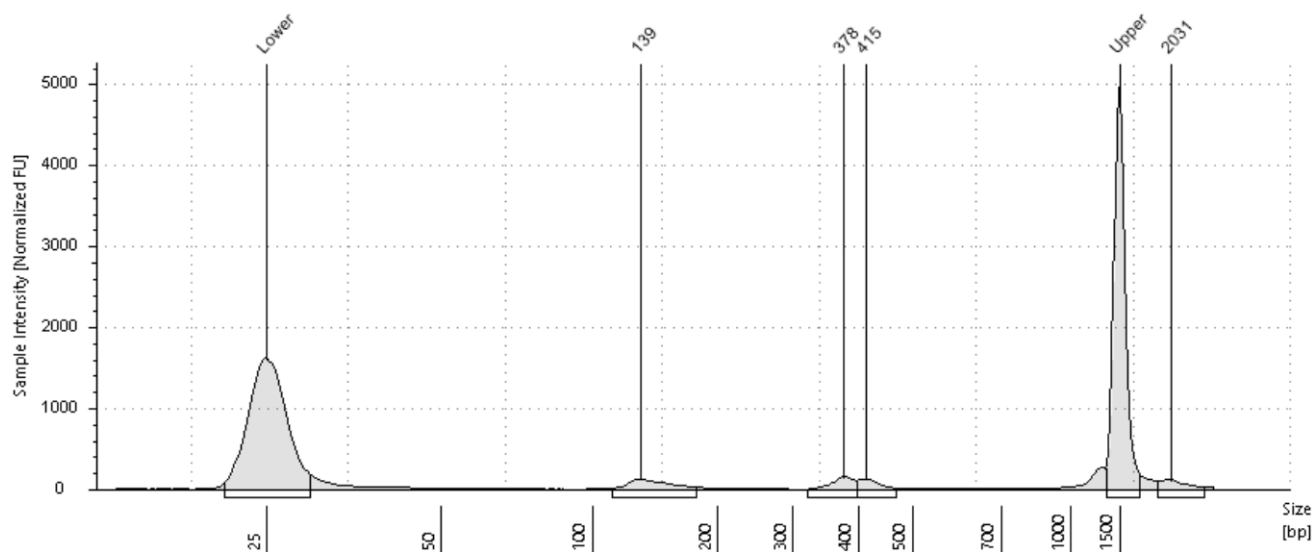


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A2	1.59	2EV3		Caution! Expired ScreenTape device; Peak out of Sizing Range

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.17	-	441	-		Lower Marker
139	0.554	-	6.11	34.86		
378	0.382	-	1.56	24.04		
415	0.297	-	1.10	18.70		
1500	6.50	6.50	6.67	-		Upper Marker
2031	0.356	-	0.270	22.40		Peak outside of Sizing Range

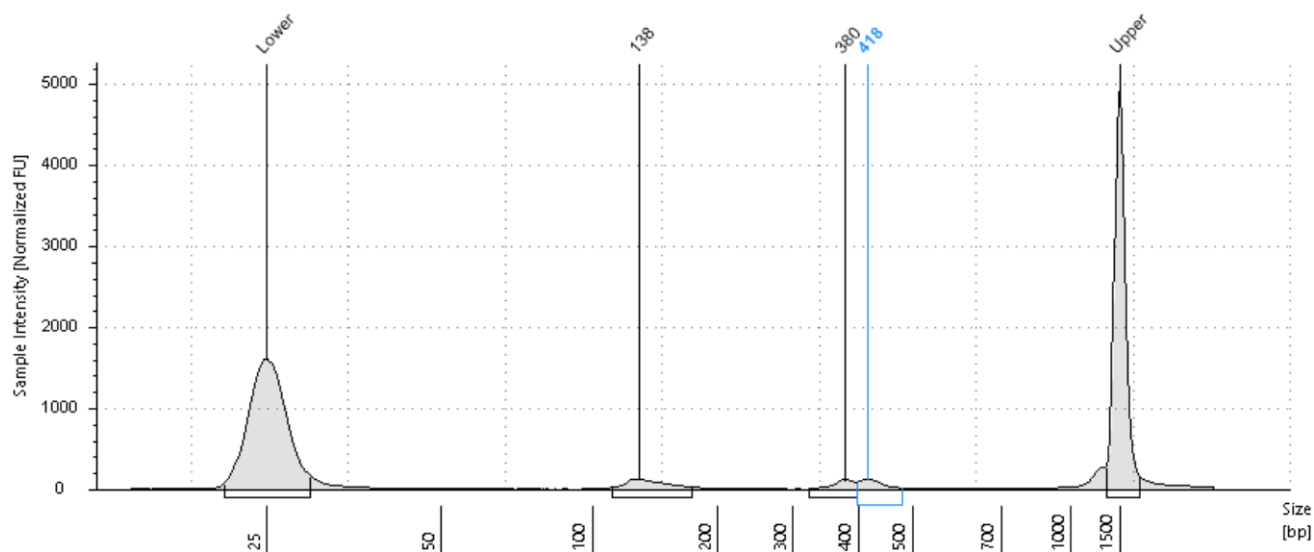
B2: 2EV30**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
B2	1.20	2EV30	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.24	-	446	-		Lower Marker
138	0.579	-	6.47	48.19		
380	0.290	-	1.17	24.11		
418	0.333	-	1.23	27.71		
1500	6.50	6.50	6.67	-		Upper Marker

C2: 2EV34

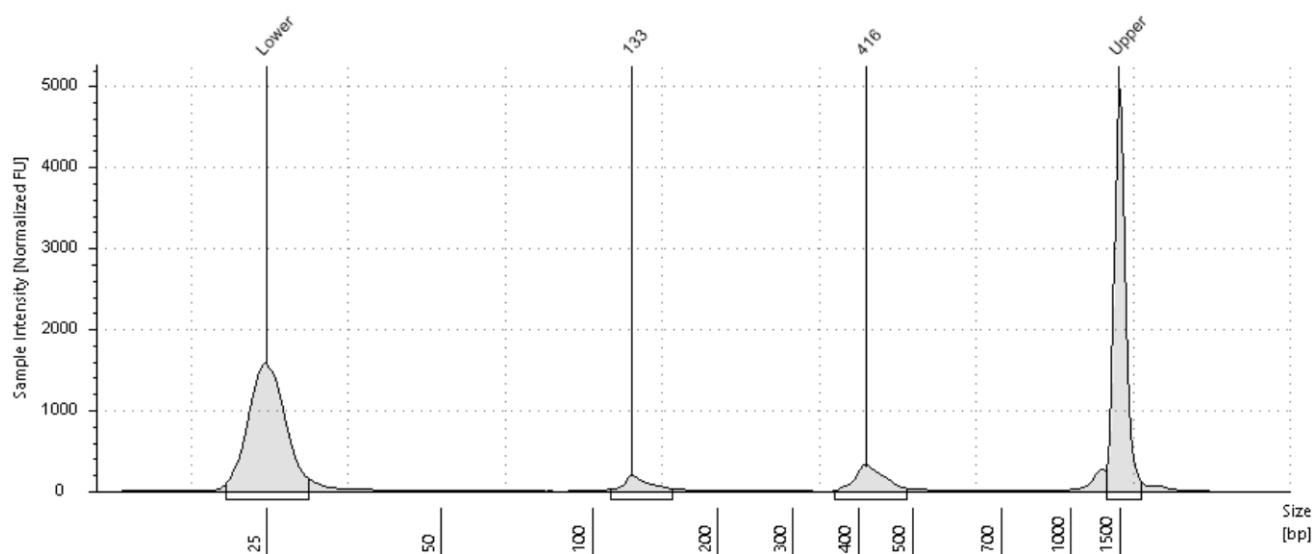


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
C2	1.66	2EV34	⚠	Caution! Expired ScreenTape device

Peak Table


Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.85	-	421	-		Lower Marker
133	0.572	-	6.64	34.54		
416	1.08	-	4.01	65.46		
1500	6.50	6.50	6.67	-		Upper Marker

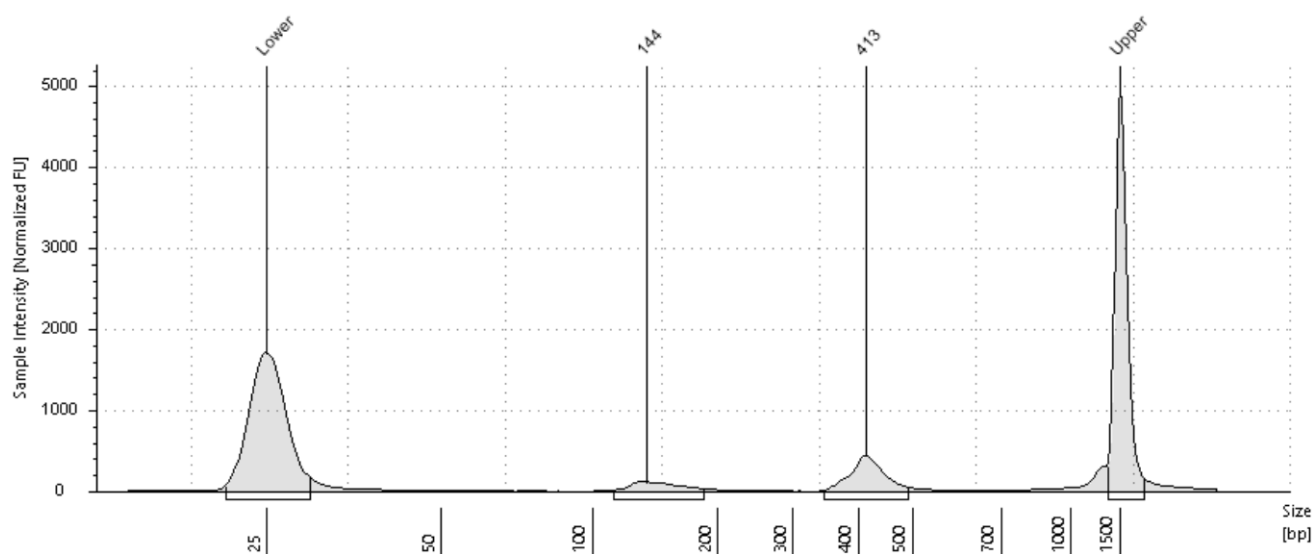D2: 2EV44**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
D2	2.12	2EV44	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.76	-	416	-		Lower Marker
144	0.592	-	6.33	27.86		
413	1.53	-	5.71	72.14		
1500	6.50	6.50	6.67	-		Upper Marker

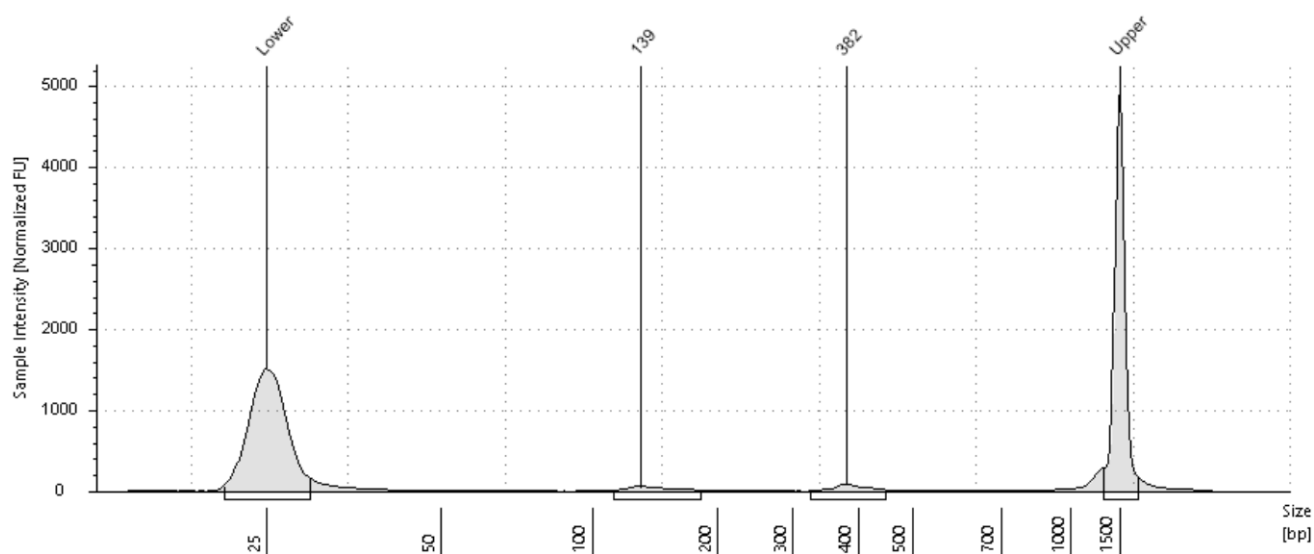
E2: 2JQ8**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
E2	0.673	2JQ8	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.39	-	455	-		Lower Marker
139	0.334	-	3.71	49.66		
382	0.339	-	1.36	50.34		
1500	6.50	6.50	6.67	-		Upper Marker

F2: 9GT46

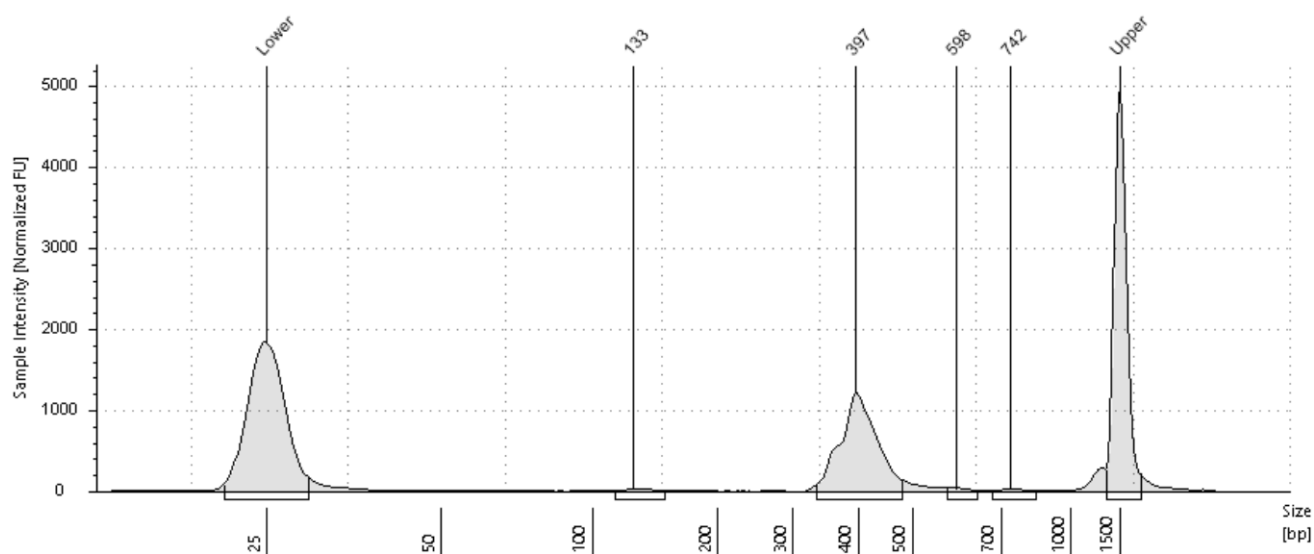


Sample Table

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
F2	4.79	9GT46	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/ul]	Assigned Conc. [ng/ul]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.29	-	448	-		Lower Marker
133	0.0810	-	0.935	1.69		
397	4.56	-	17.7	95.21		
598	0.0871	-	0.224	1.82		
742	0.0611	-	0.127	1.28		
1500	6.50	6.50	6.67	-		Upper Marker

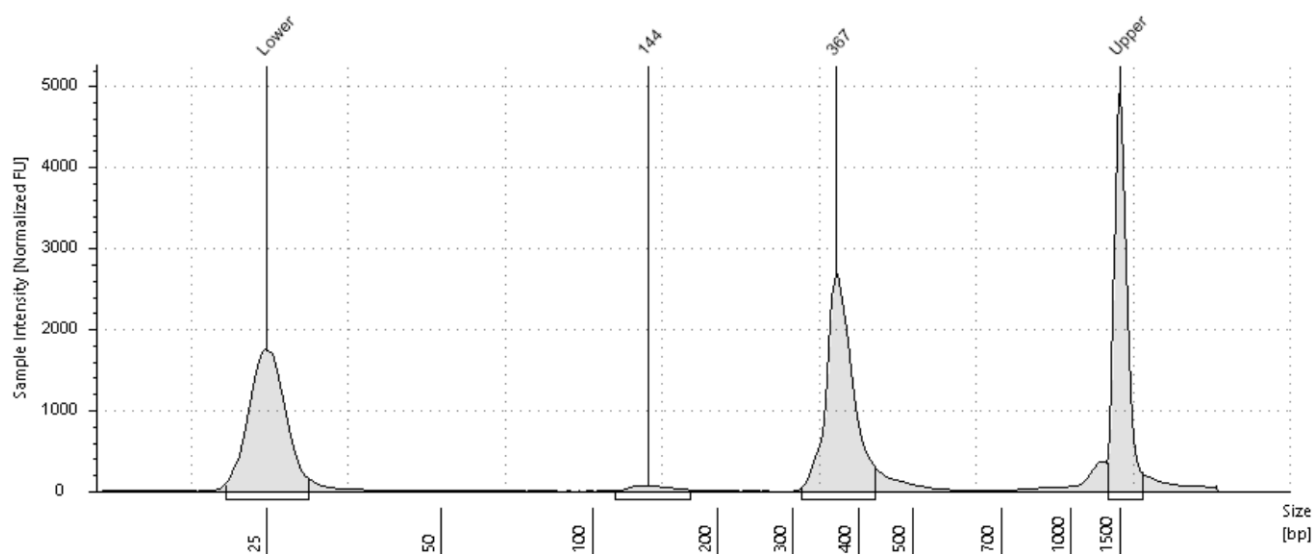
G2: 4DW11**Sample Table**

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
G2	7.49	4DW11	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	6.76	-	416	-		Lower Marker
144	0.284	-	3.03	3.79		
367	7.20	-	30.2	96.21		
1500	6.50	6.50	6.67	-		Upper Marker

H2: 4EV14

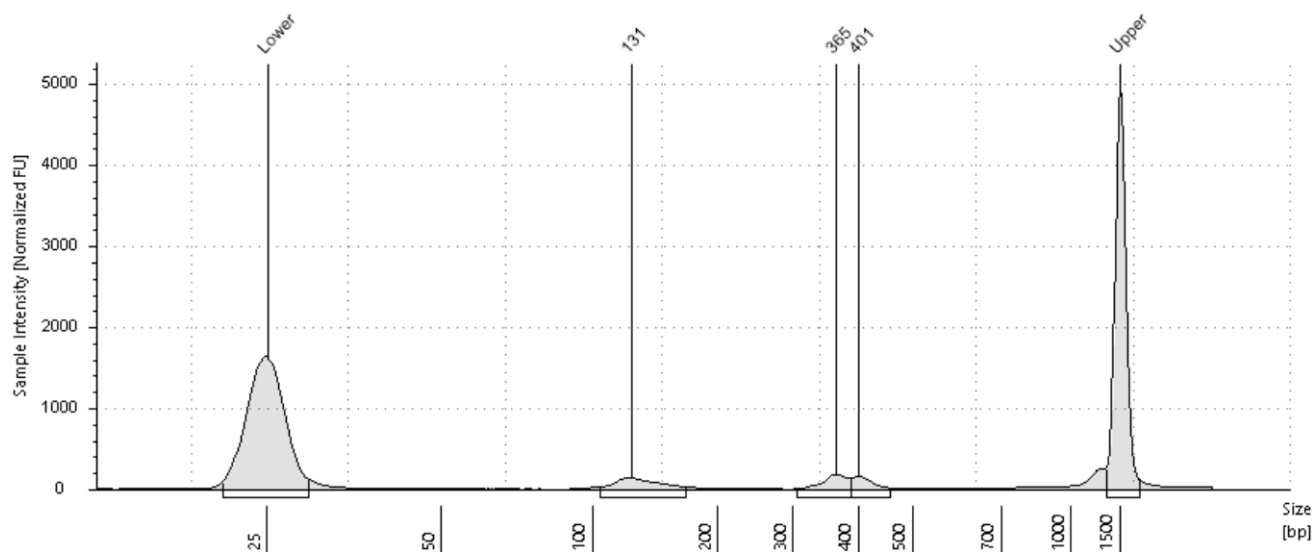

Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
H2	1.59	4EV14	⚠	Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	7.47	-	460	-		Lower Marker
131	0.698	-	8.22	43.93		
365	0.508	-	2.14	31.99		
401	0.383	-	1.47	24.08		
1500	6.50	6.50	6.67	-		Upper Marker