Data-dependent acquisition [DDA]

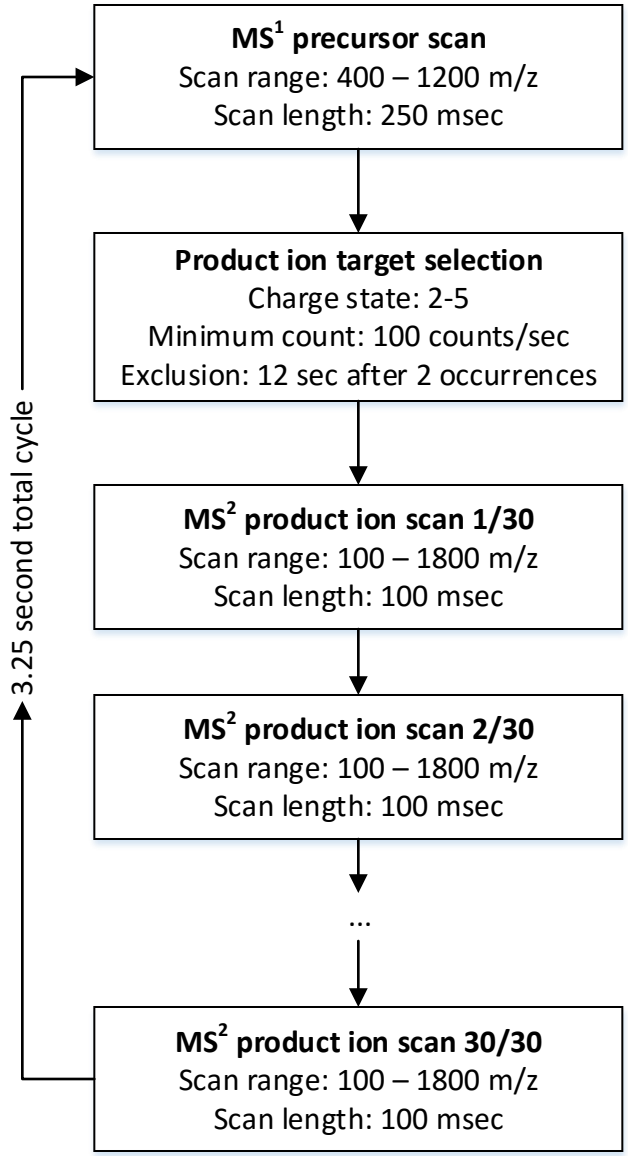

SWATH data-independent acquisition [DIA]

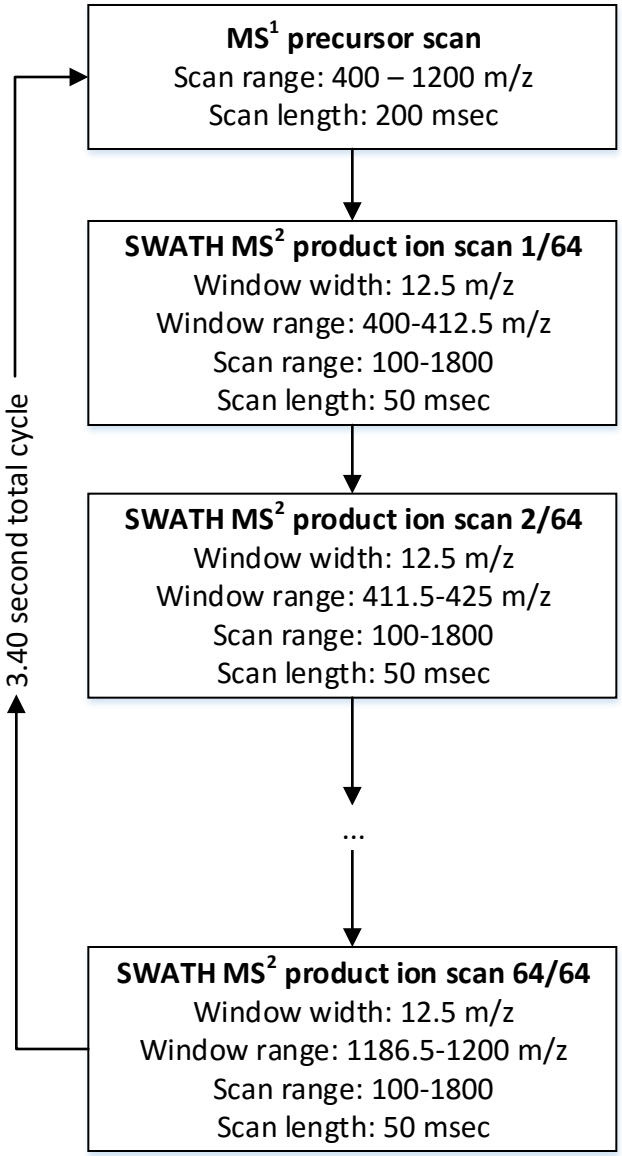

*** 120 minute gradient**

*** Chromatographic peak width ~ 30 seconds**