

GENX2 Porewater SO₄/Cl

2025 Samples Run 3

Date QAQC'd: 2025-10-02

Contents

0.1	Run Information	2
0.2	Assess Standard Curves	3
0.3	Assess Check Standards	4
0.4	Assess Blanks	5
0.5	Assess Duplicates	7
0.6	Calculate mmol/L concentrations & salinity, add dilutions	8
0.7	Assess Analytical Spikes	9
0.8	Check if samples within the range of the standard curve	9
0.9	Export Processed Data	10

##Add Required Packages

0.1 Run Information

```
##### Run information - PLEASE CHANGE
Date_Run = "2025-09-18" #Date that instrument was run
Year_run = "2025" #Year that instrument was run
Run_by = "Zoe Read" #Instrument user
Script_run_by = "Zoe Read" #Code user
run_notes = "Chk std 1 S04 is slightly lower than the expected concentration.
One dup (185_GX2_50143) had high CV.
166_GX2_50116 was above the S04 detection limit (24.5 ppm vs the 20 ppm detection limit)
" #any notes from the run

##### File Names - PLEASE CHANGE
#file path and name for raw summary data file
raw_file_name_cl = "Raw Data/GenX2_Mesocosms2025_PW_Run3_20250918_Cl.txt"
raw_file_name_so4 = "Raw Data/GenX2_Mesocosms2025_PW_Run3_20250918_S04.txt"

#file path and name of processed data file
processed_file_name = "Processed Data/GenX2_Mesocosms2025_PW_Processed_Cl_S04_Run3_20250918.csv"

##### Log Files - PLEASE CHECK
#downloaded metadata csv of dilutions
Raw_Metadata = "Raw Data/GenX2_Mesocosms2025_PW_Dilutions.csv"

#qaqc log file path for this year
Log_path = "Raw Data/COMPASS_Synoptic_Cl_S04_QAQClog_2024.csv"
```


##Set Up Code - constants and QAQC cutoffs

##Read in metadata and create similar sample IDs for matching to samples


##Import Sample Data

0.2 Assess Standard Curves


Chloride Std Curve

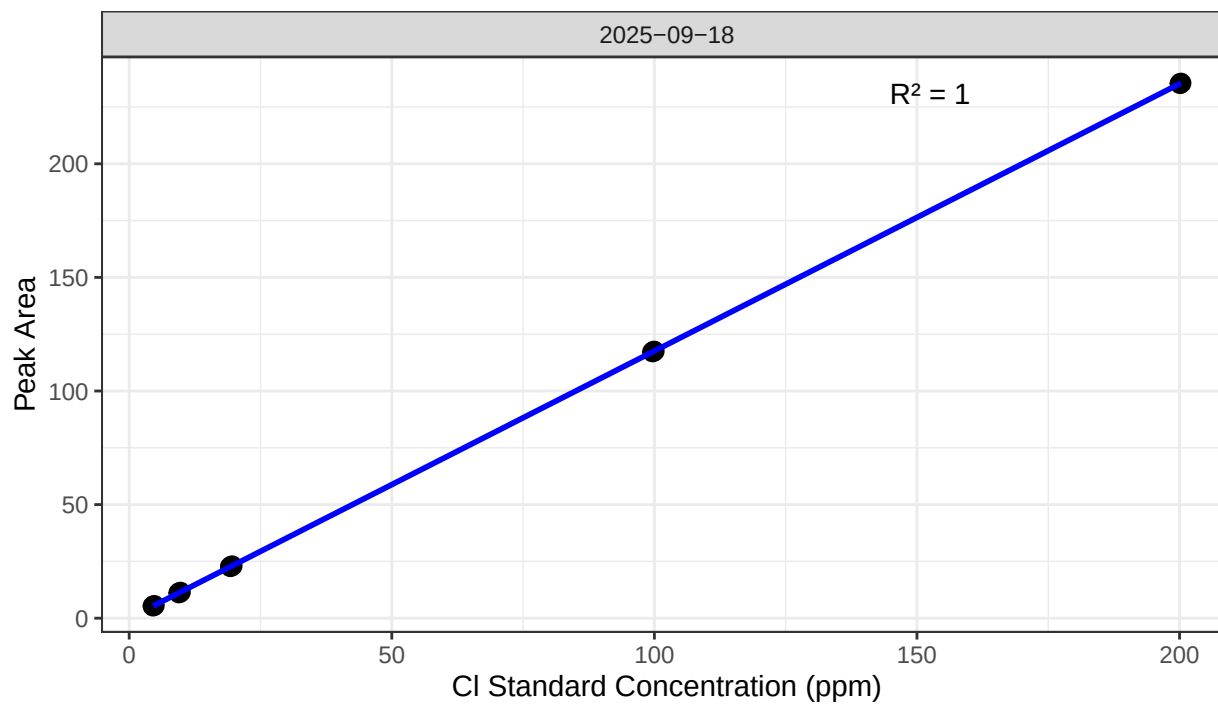

Sulfate Std Curve

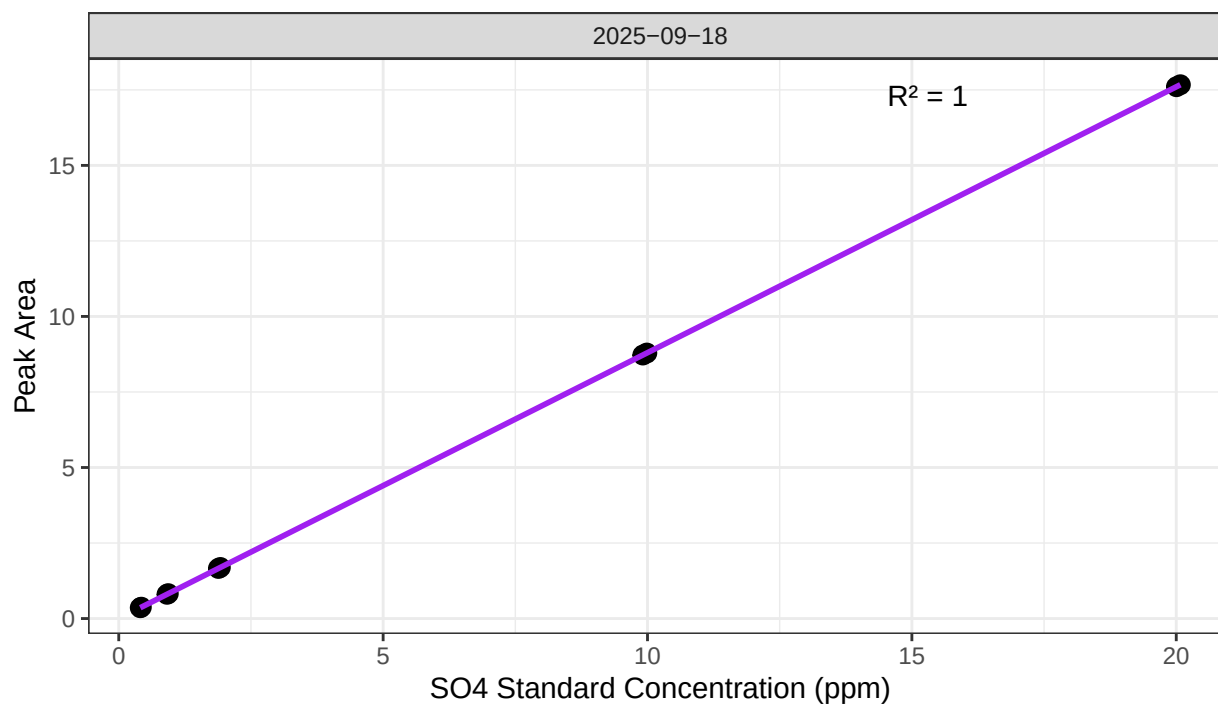

```
## [1] "QAQC log file exists and has been read into the code."
```

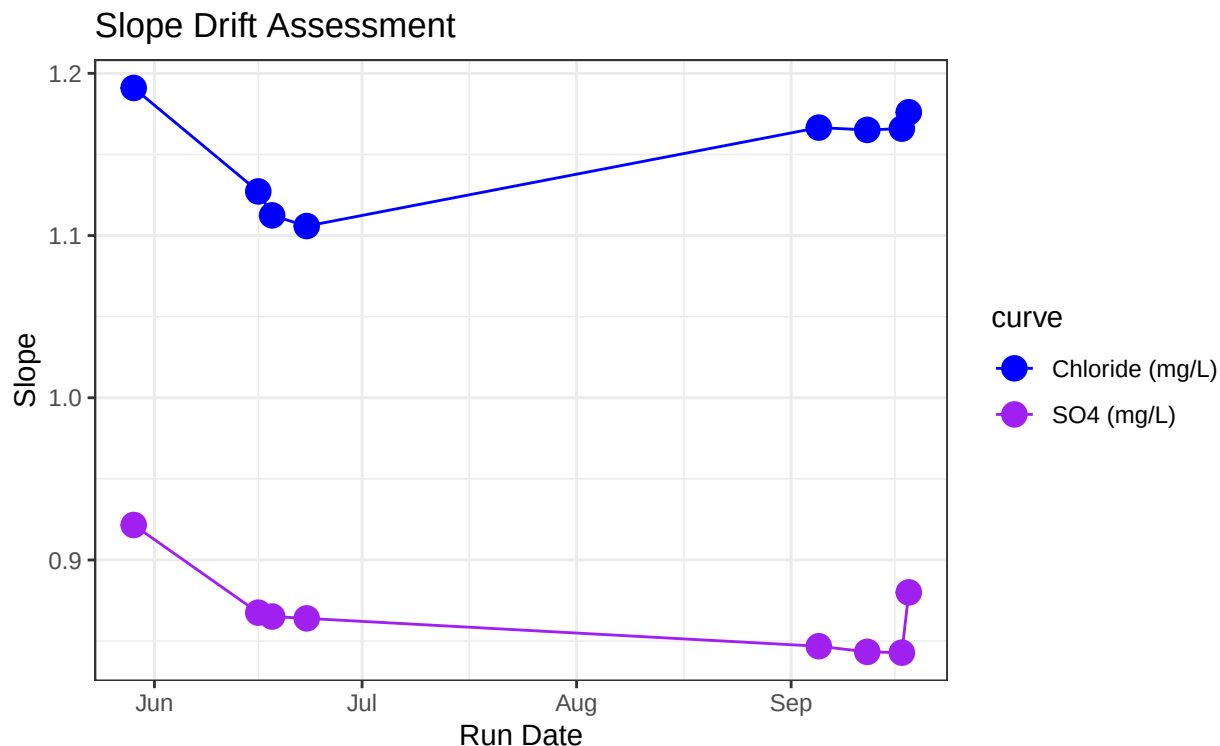

```
## [1] "Cl Curve r2 GOOD"
```

```
## [1] "SO4 Curve r2 GOOD"
```


0.3 Assess Check Standards

```
## # A tibble: 5 x 5
##   sample_ID mean_Cl sd_Cl   cv_Cl flag_Cl
##   <chr>      <dbl> <dbl>   <dbl> <chr>
## 1 Standard 1    4.71 0.122 0.0258 Chloride Check Standard RSD within Range - ~
## 2 Standard 2    9.67 0.144 0.0149 Chloride Check Standard RSD within Range - ~
## 3 Standard 3   19.5 0.147 0.00752 Chloride Check Standard RSD within Range - ~
## 4 Standard 4  100. 0.217 0.00218 Chloride Check Standard RSD within Range - ~
## 5 Standard 5  200. 0.130 0.000652 Chloride Check Standard RSD within Range - ~
```

```
## # A tibble: 5 x 5
##   sample_ID mean_SO4 sd_SO4   cv_SO4 flag_SO4
##   <chr>      <dbl> <dbl>   <dbl> <chr>
## 1 Standard 1    0.419 0.00860 0.0205 Sulfate Check Standard RSD within Range --
## 2 Standard 2    0.928 0.0104 0.0112 Sulfate Check Standard RSD within Range --
## 3 Standard 3    1.91 0.0157 0.00823 Sulfate Check Standard RSD within Range --
## 4 Standard 4    9.98 0.0454 0.00455 Sulfate Check Standard RSD within Range --
## 5 Standard 5   20.0 0.0524 0.00261 Sulfate Check Standard RSD within Range --
```

```
## [1] ">80% of Chloride Check Standards have RSD within range - PROCEED"
```

```
## [1] ">80% of Sulfate Check Standards have RSD within range - PROCEED"
```

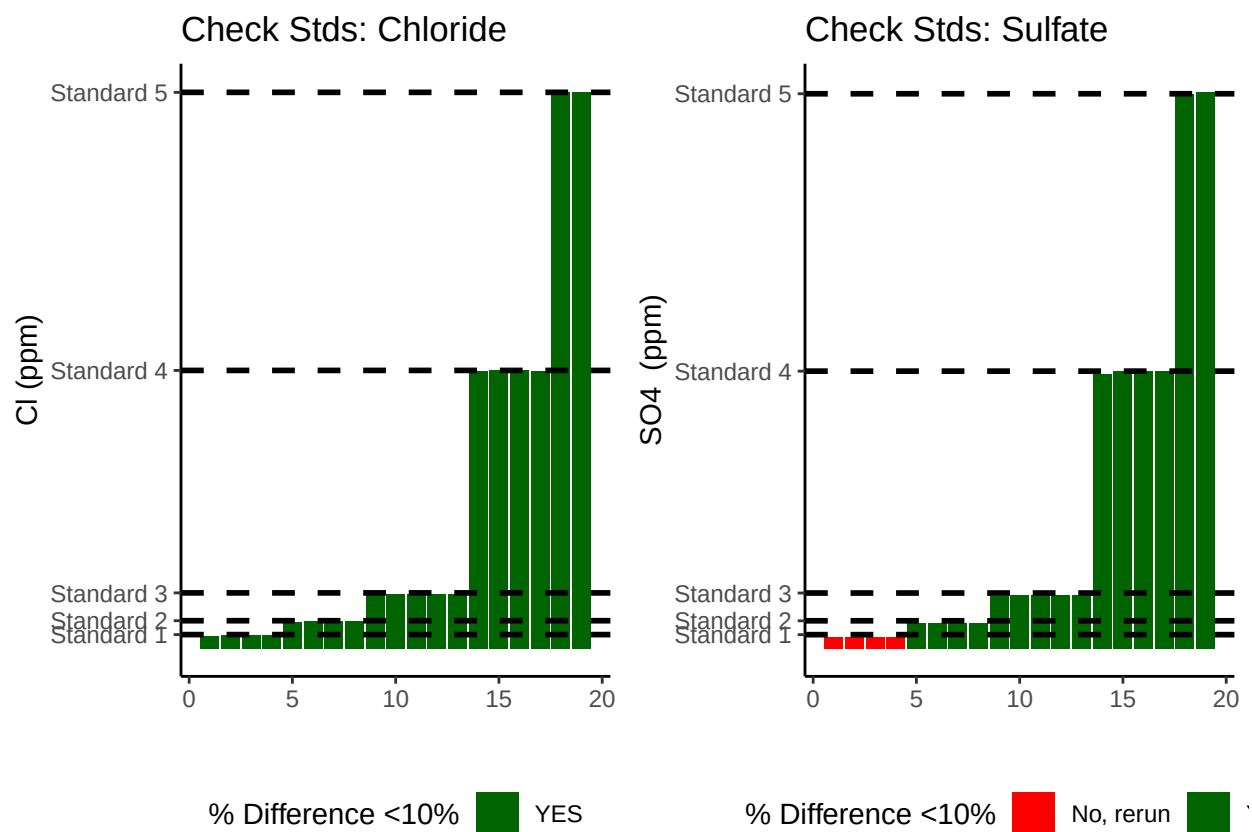


```
## [1] ">80% of Chloride Check Standards are within range of expected concentration - PROCEED"
```

```
## [1] "<80% of Sulfate Check Standards are within range of expected concentration - REASSESS"
```

0.4 Assess Blanks

```
## [1] ">80% of Chloride Blank concentrations are lower 25% quartile of samples"
```

```
## [1] ">80% of Sulfate Blank concentrations are lower 25% quartile of samples"
```

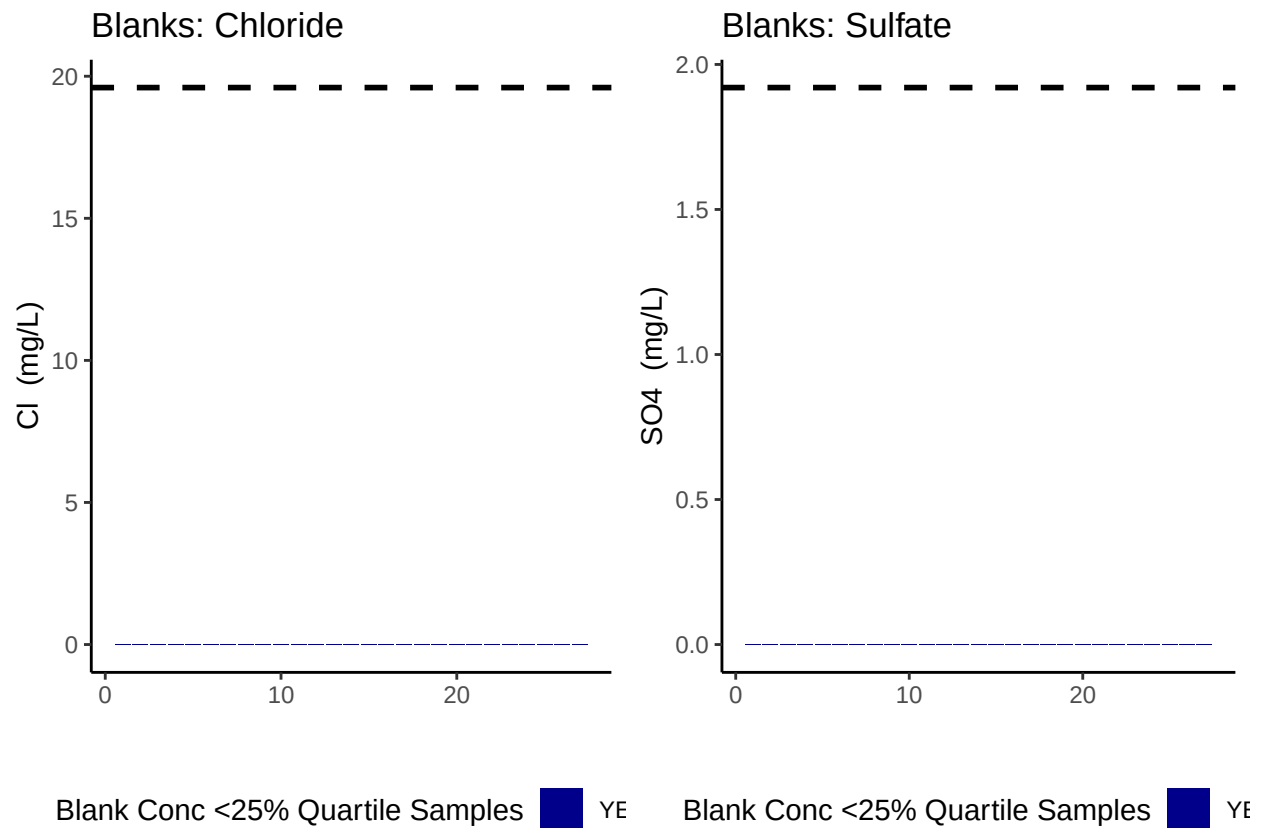


```
## Chloride blanks mean ppm:
```

```
## [1] 0.002111111
```

```
## Sulfate blanks mean ppm:
```


```
## [1] 0
```

0.5 Assess Duplicates

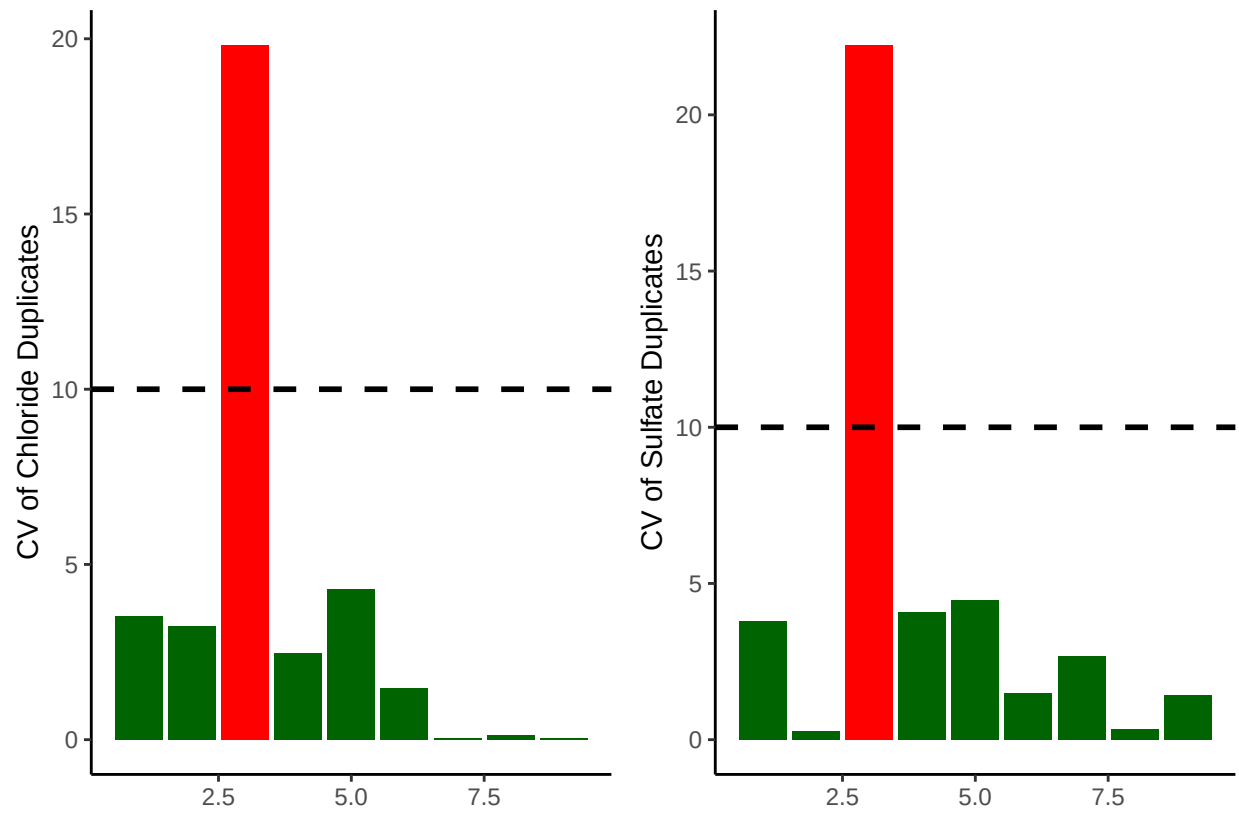

```
## [1] ">80% of Chloride Duplicates have a CV <10% - PROCEED"
```

```
## [1] ">80% of Sulfate Duplicates have a CV <10% - PROCEED"
```

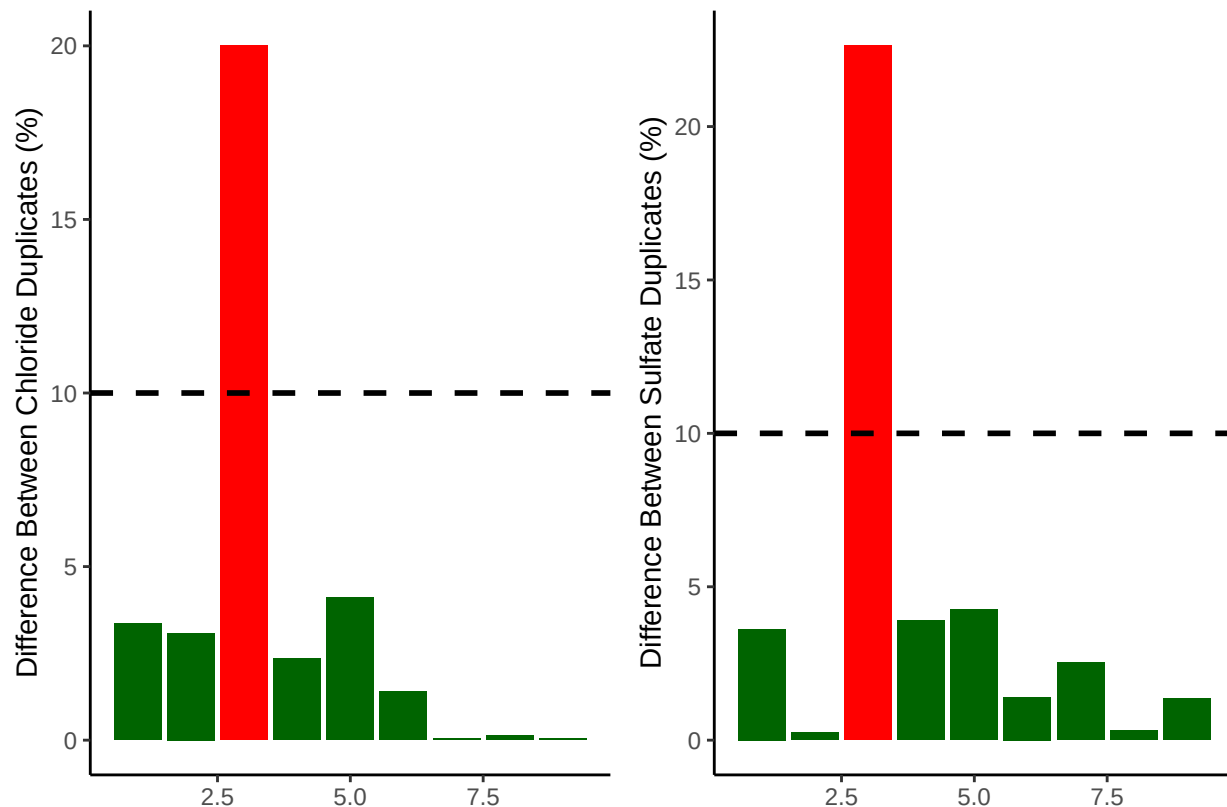

```
## [1] ">80% of Chloride Duplicates have a percent difference <10% - PROCEED"
```

```
## [1] ">80% of Sulfate Duplicates have a percent difference <10% - PROCEED"
```

0.6 Calculate mmol/L concentrations & salinity, add dilutions

```
# Convert ppm to mmol/L
all_dat$S04_Conc_mM <- (all_dat$S04_ppm / s_mw)
all_dat$Cl_Conc_mM <- (all_dat$Cl_ppm / cl_mw)

# Calculate Salinity
# calculated using the Knudsen equation
# Salinity = 0.03 + 1.8050 * Chlorinity
# Ref: A Practical Handbook of Seawater Analysis by Strickland & Parsons (P. 11)
# =((1.807*Cl_ppm)+0.026)/1000
all_dat$salinity <- ((1.8070 * all_dat$Cl_ppm) + 0.026) / 1000

#Need to determine dilution factors for your samples

#Separate namings
all_dat <- all_dat %>%
  mutate(sample_ID_long = sample_ID) %>%
  separate(sample_ID_long, into = c("number", "project", "ID", "test"), sep = "_") %>%
  mutate(sample_ID_short = paste(number, project, ID, sep = "_"))
```




```
## Warning: Expected 4 pieces. Missing pieces filled with 'NA' in 133 rows [1, 2, 3, 4, 5,
## 6, 7, 8, 9, 10, 11, 12, 13, 14, 15, 16, 17, 18, 19, 20, ...].
```

```
#merge dilution with sample run data
```

```
merged_data <- all_dat %>%
```

```
  left_join(dionex_metadata, by = c("sample_ID_short" = "Cl_S04_ID"))
```

0.7 Assess Analytical Spikes

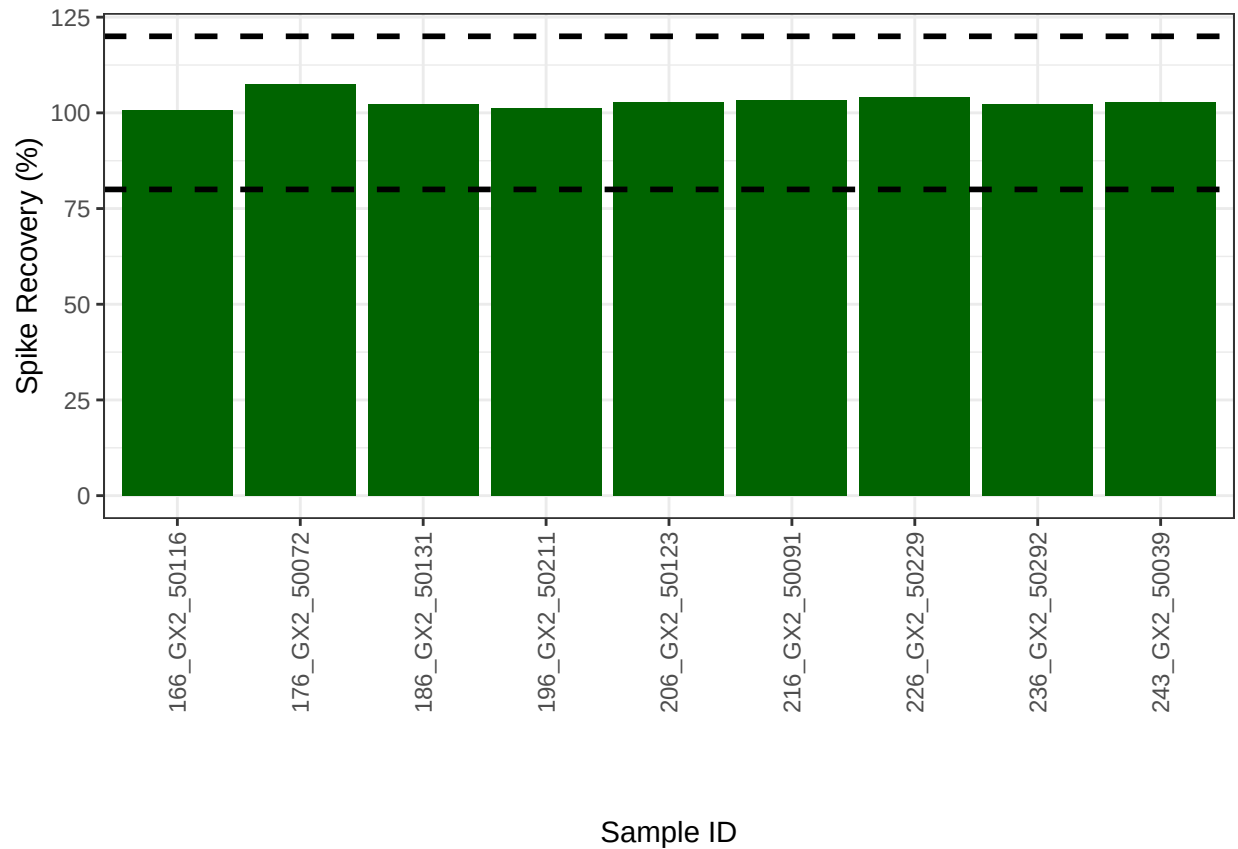

```
## [1] ">80% of S04 spikes have a recovery between the high and low cutoff - PROCEED"
```

0.8 Check if samples within the range of the standard curve

```
## Sample Flagging
```

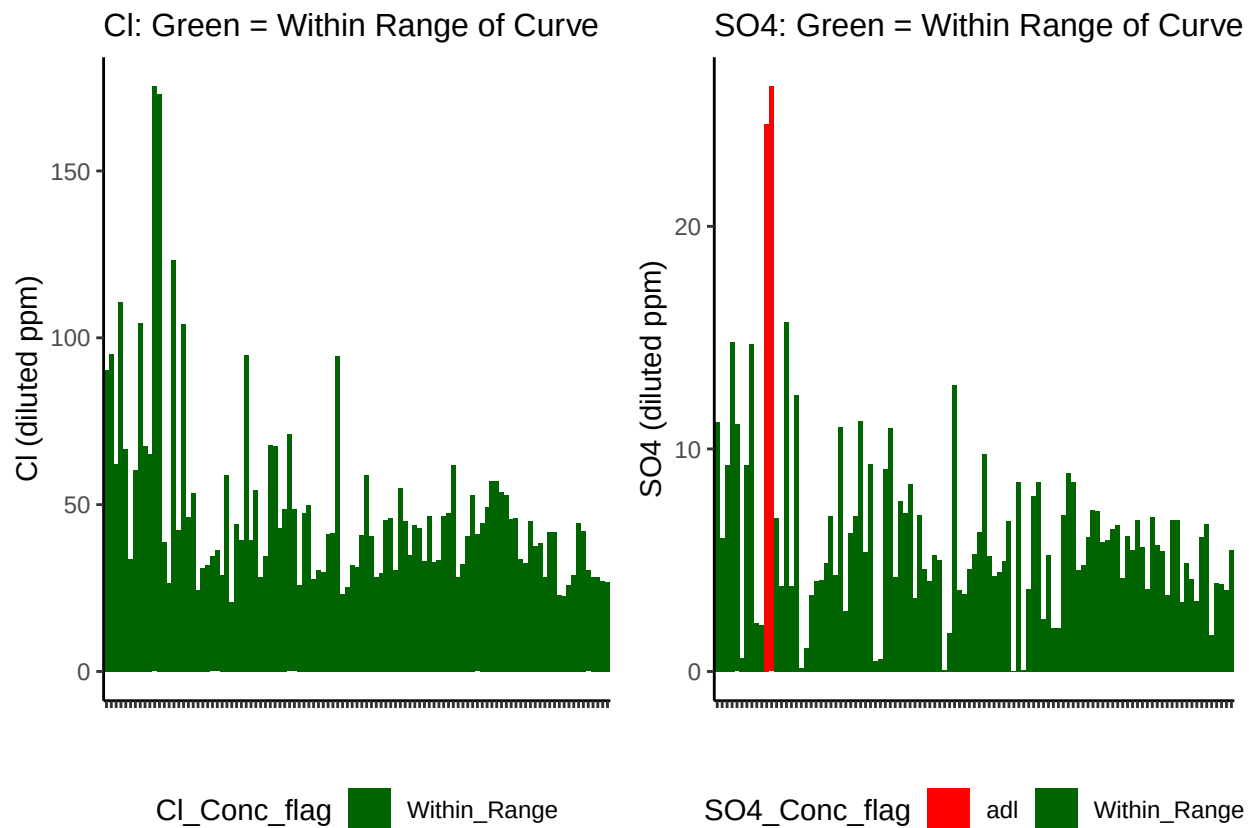


Table 1: SO4 samples

SO4_Conc_flag	Percent_samples
Within_Range	98.095238
adl	1.904762

Table 2: Cl samples

Cl_Conc_flag	Percent_samples
Within_Range	100

0.9 Export Processed Data

#end