

Titration report

LabX

Method

Method ID	SERCCAL RICCA 3 Points	Release state	Released
Name	Calibration	Modified by	SystemInternal
Modified on	2/21/2023 9:53:01 AM		

Summary

Samples

	Sample ID	Name	Result	State
1	RICCA HIGH PRES	pH	4.000	
2	RICCA HIGH PRES	pH	7.000	
3	RICCA HIGH PRES	pH	10.000	


Results

Zero point 1 Cal1.Z1 6.935 pH
Slope 1 Cal1.S1 -58.90 mV/pH

Calibration

Sensor Sensor DG115-SC
Creation time 2/20/2024 11:25:25 AM
Successful Yes
Calib. temperature 24.6 °C
SLOPECal -58.90 mV/pH
ZEROCal 6.935 pH

Calibration Curve

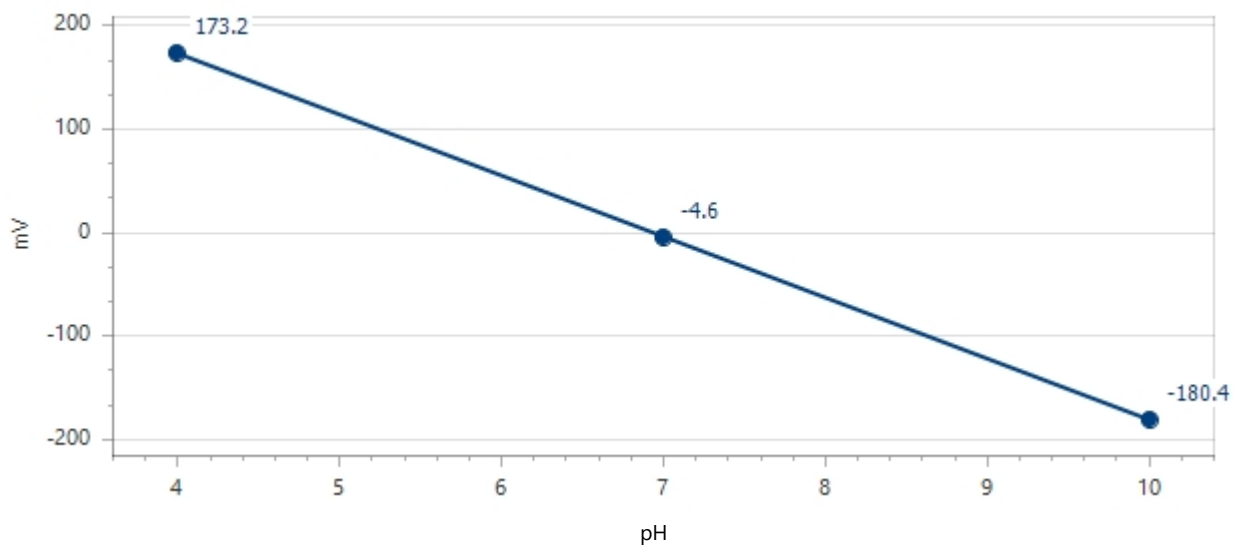

Used Instruments

Name	SERCtitrate	Serial number	B433917554
------	-------------	---------------	------------

Titration report



Responsible User

Time	Login name	Full name
2/20/2024 11:18:33 AM	SystemInternal	System internal account