

Sign In CURIE

Username

Password


Remember me


Sign In

Have problems? <u>Contact Us</u>.

CURIE System

Guide Better. Treat Better.

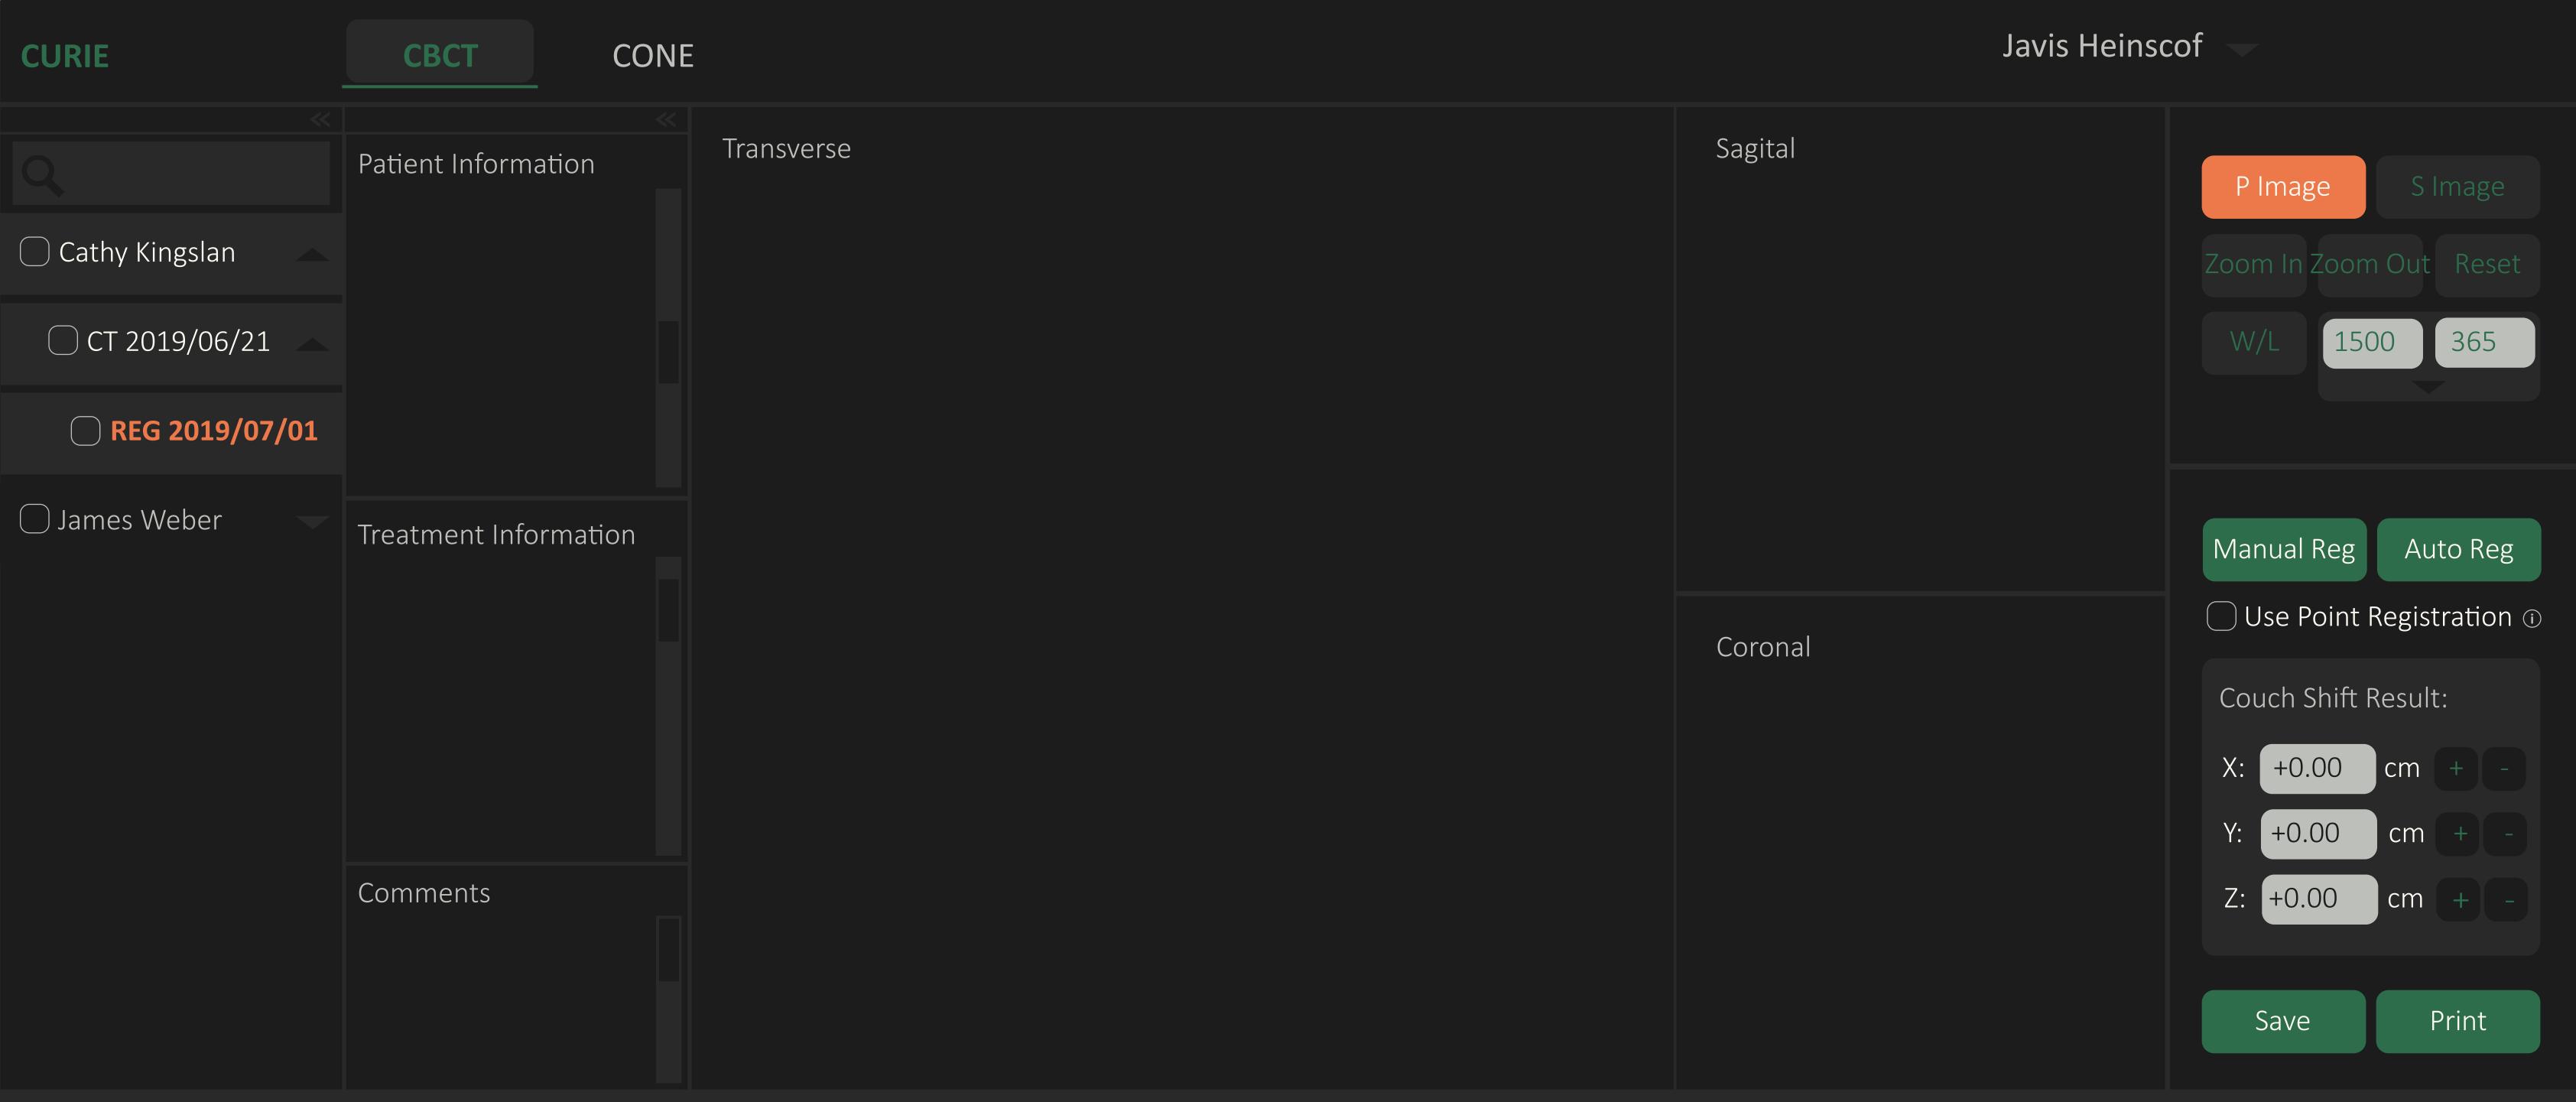

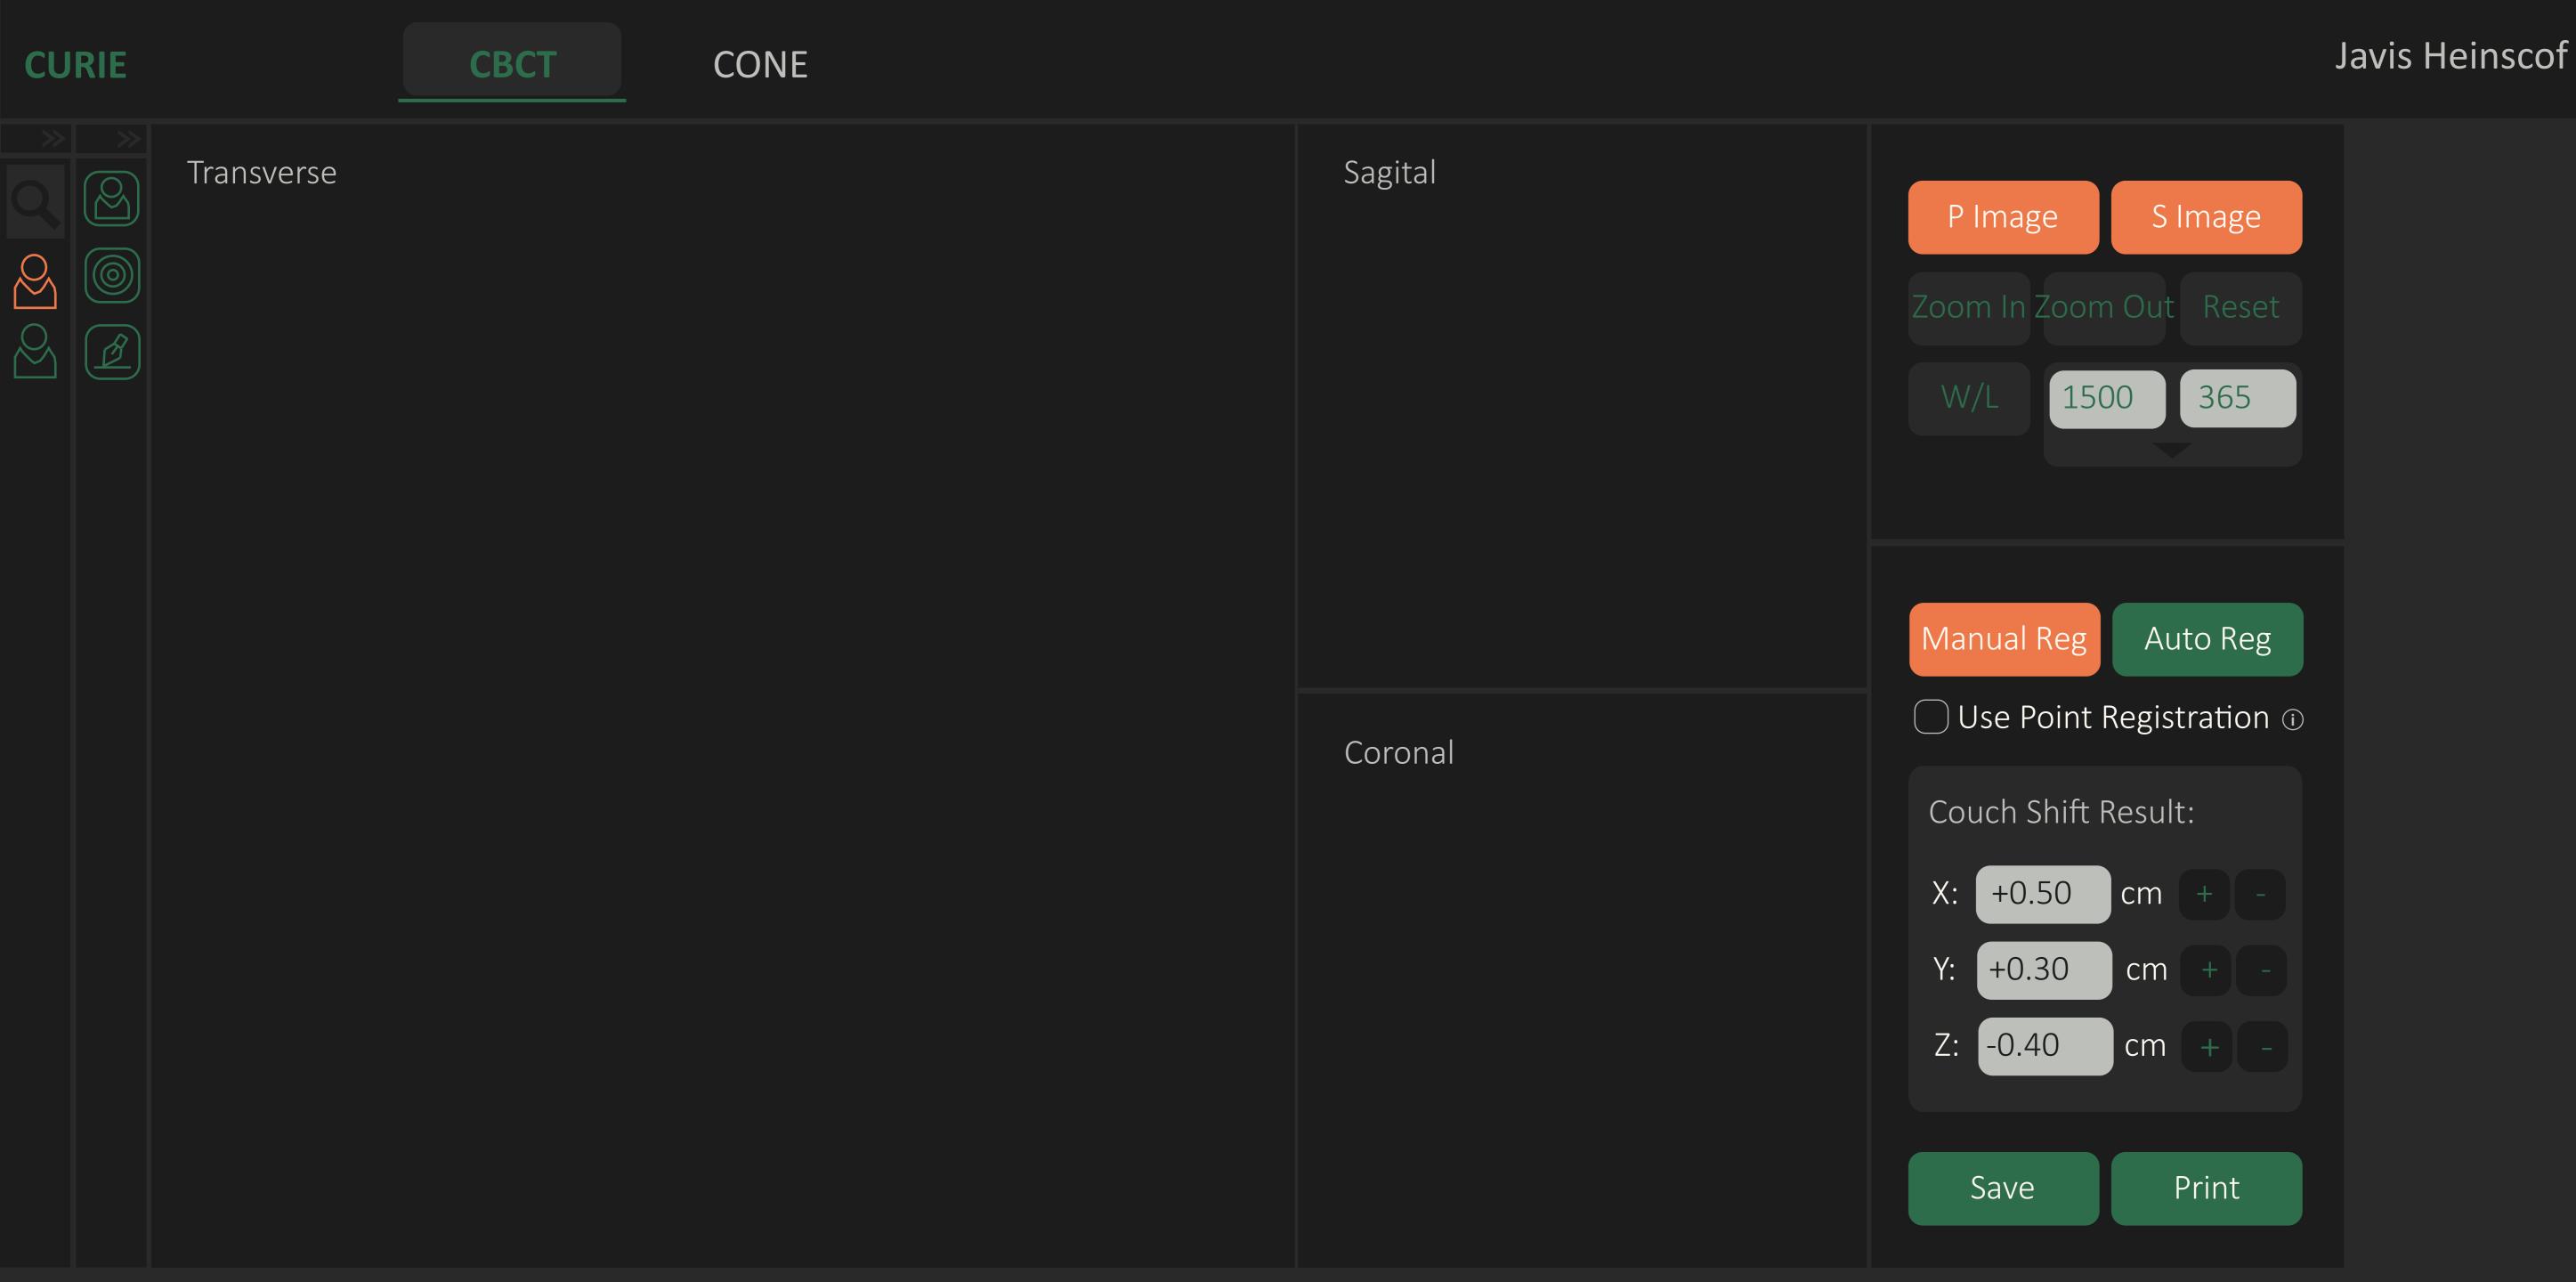

Tolerance

Image Acquisition

Hot-Keys

Limitation Range:

1000

1100

cm (?)


Tolerance:

1000

1100 ~

cm ?

Save

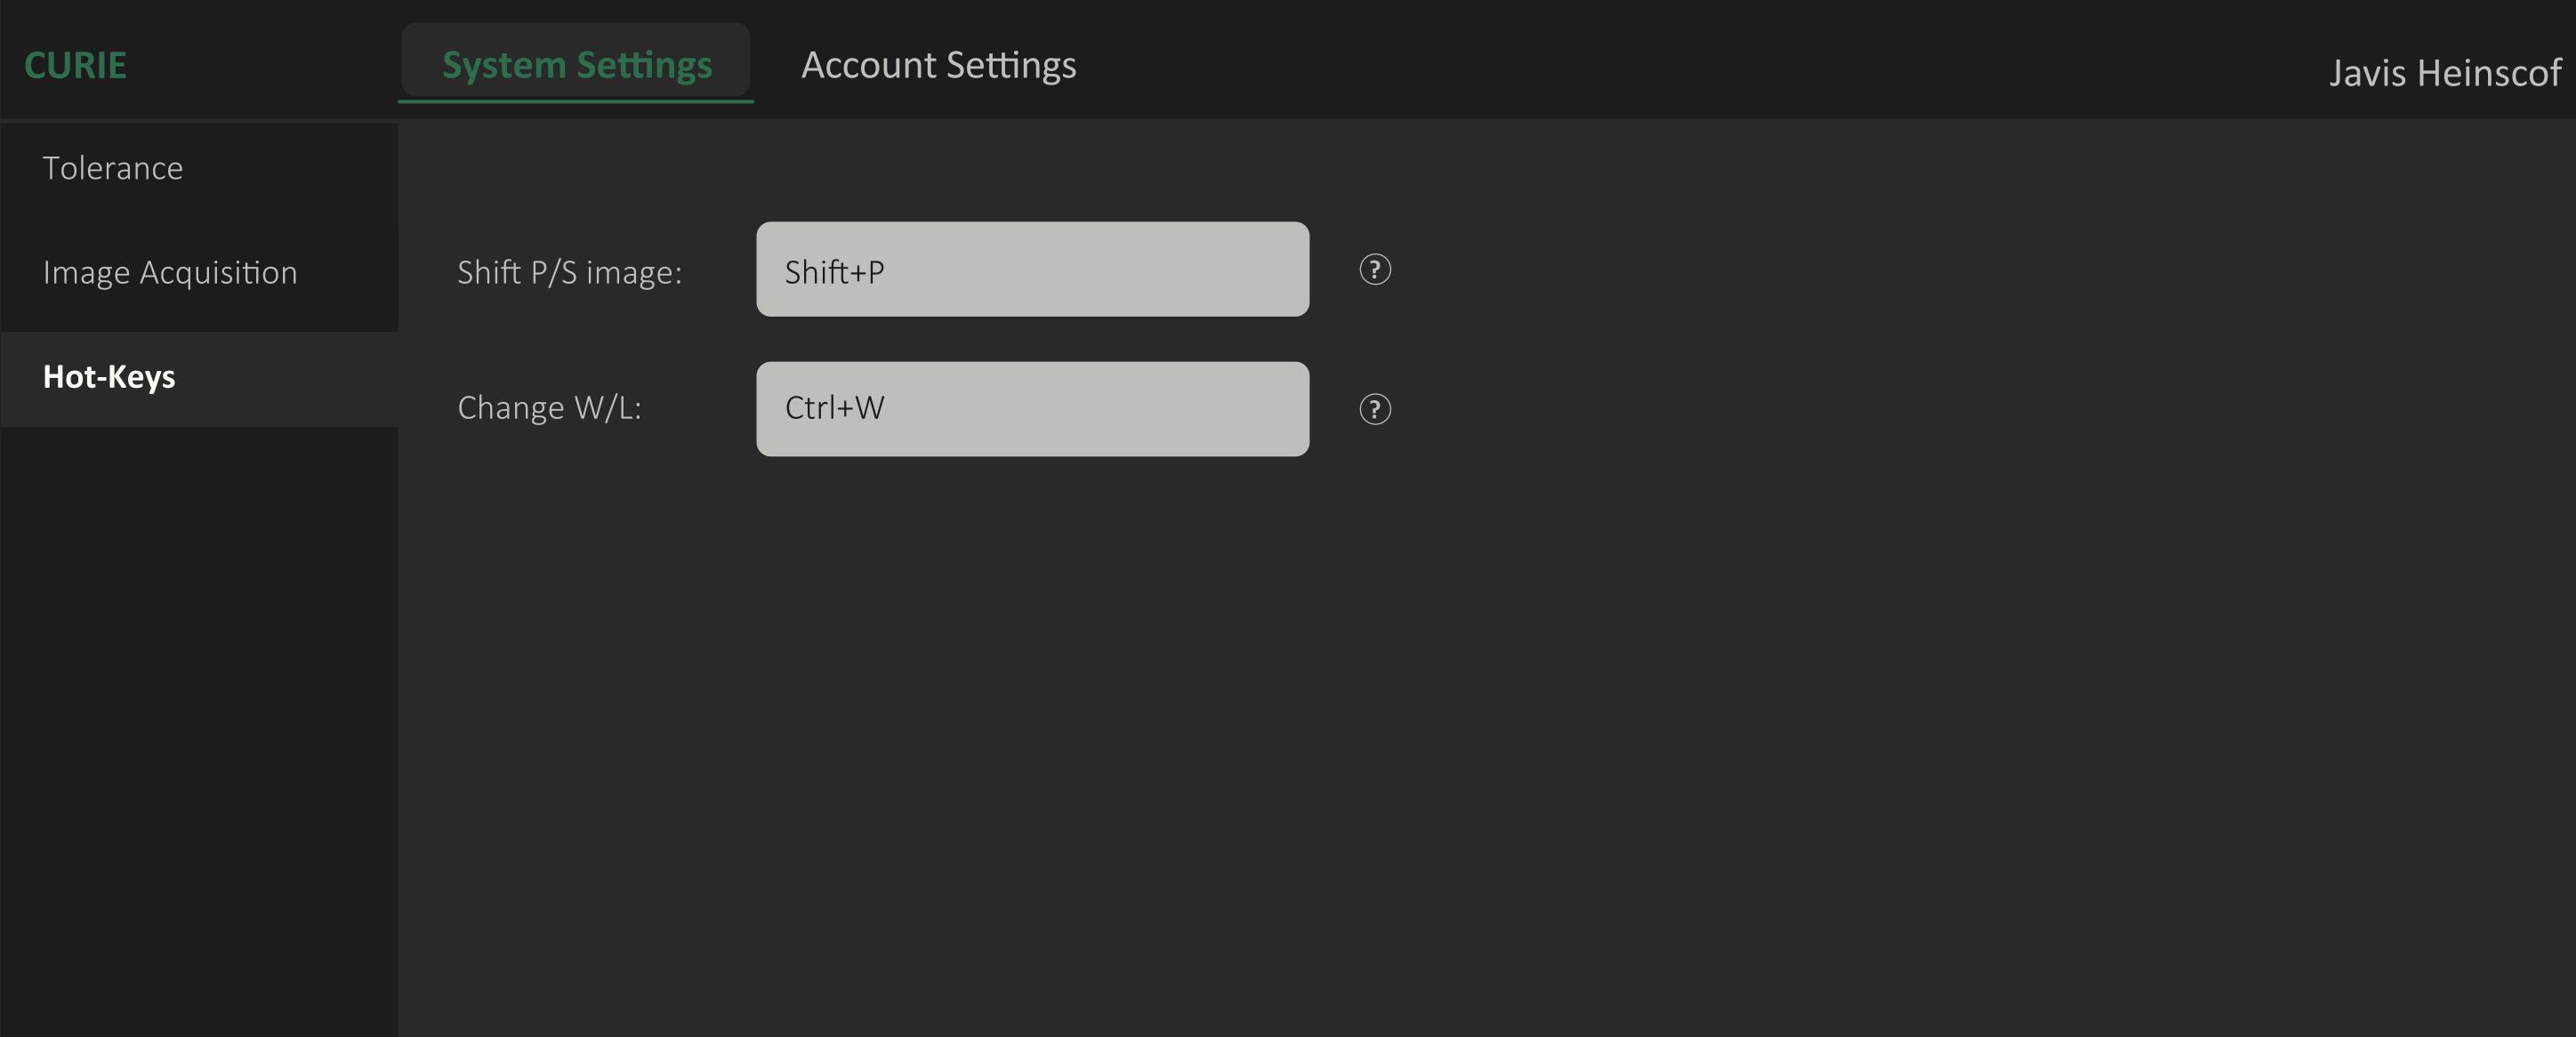

Save

Javis Heinscof

System Settings

Account Settings

Sign Out

W/L

1500

365

Preset: Bone

Preset: Brain

Preset: Lung

Role Assignment:


Administrator

Administrator

Physician

Physicist

Javis Heinscof

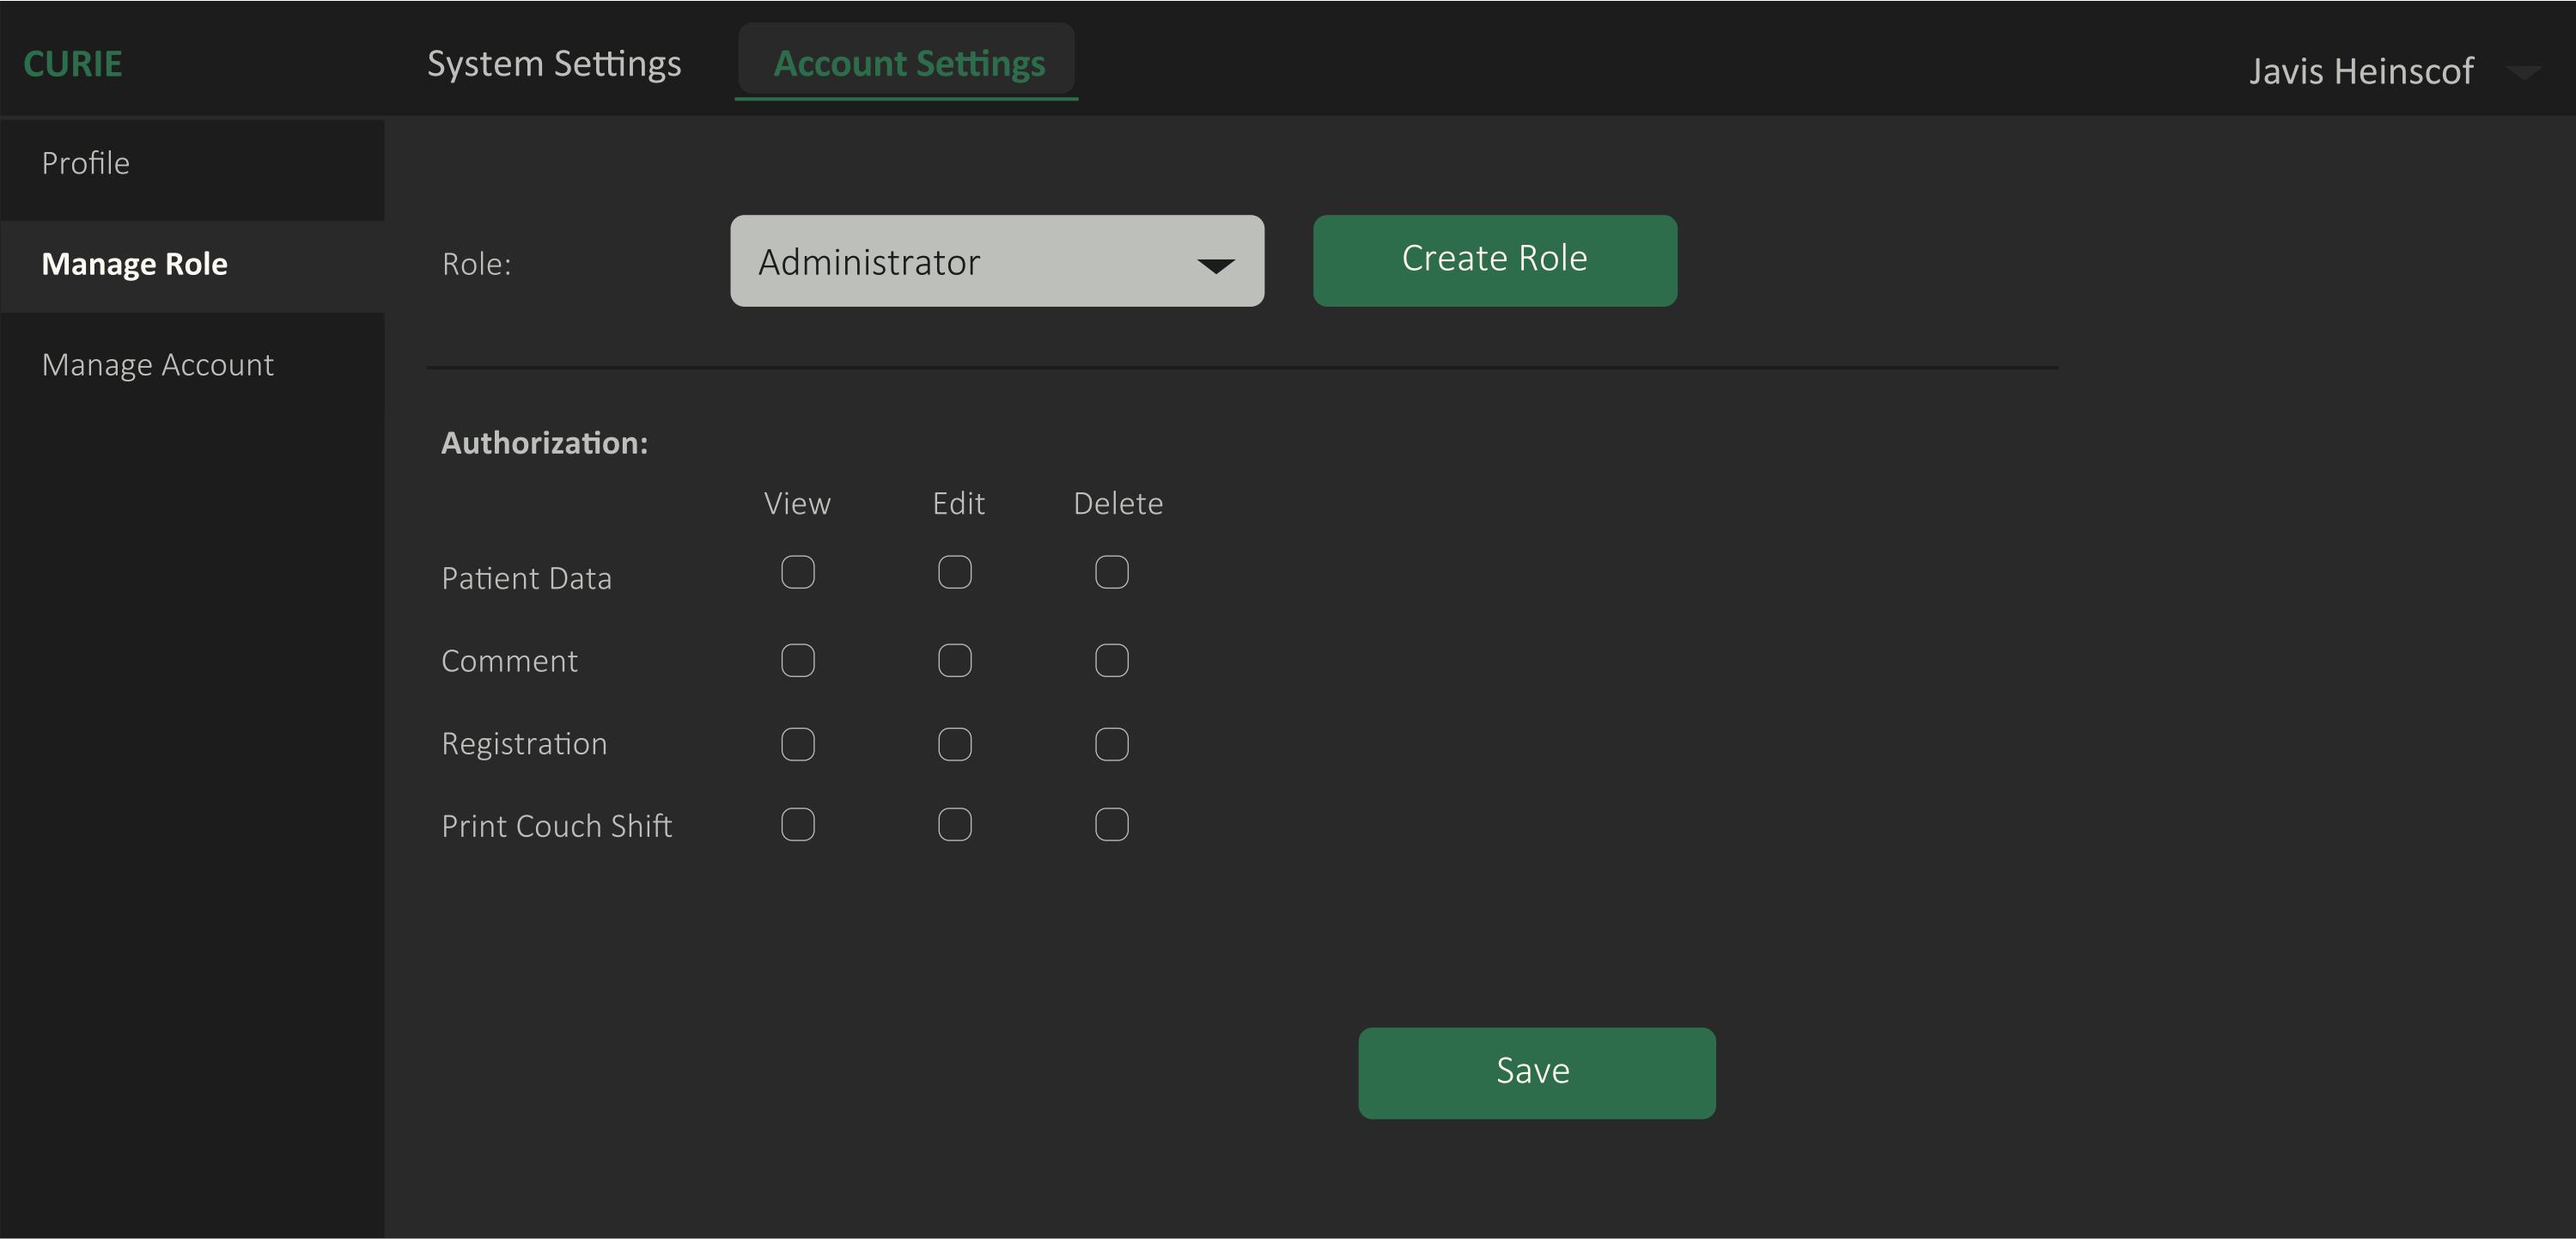

User Name:

Full Name:

JavisH

Javis Heinscof

Email:

JavisHeinscof@TeckTron.com

Department:

Cancer Department

Role Assignment:

Administrator

Reset Password

Save