

Certificate of Calibration

INSTRUMENT

Model Number: iPA-0850A
Serial Number: TX2152400189
Description: PORTABLE IM TEST SET-850MHz iPA-0850A

CERTIFICATION

Calibration Date: April 04 2023
Location of Calibration: 29 Smallwood Place, Murarrie, QLD, 4172, Australia

This document certifies that the instrument detailed above is in conformance with the manufacturer's specifications, which can be accessed on the web address of <http://www.kaelus.com/test-and-measurement-solutions/>.

All calibrations were conducted in a laboratory environment at or around +25° Celsius, using test equipment calibrated against national and/or international standards.

PIM equipment calibration and measurements are conducted in accordance with IEC62037. Kaelus is an ISO9001 certified company and all documentation complies with this standard

Kaelus recommends a calibration interval of 12 months to ensure measurement accuracy. The next recommended calibration date is 04 Apr 2024

Issued By: Technical Supervisor

Approved By: Quality Manager

Customer Test Report

PRODUCT

Model Number : iPA-0850A
Serial Number : TX2152400189
Description : PORTABLE IM TEST SET-850MHz iPA-0850A

TEST DATA

Verification Date : 05 Apr 2023
Testing Location : 29 Smallwood Place, Murarrie, QLD, 4172, Australia

This document certifies that the instrument detailed above is in conformance with the manufacturer's specifications, which can be accessed on the web address of <http://www.kaelus.com/rf-conditioning-solutions/>.

All calibrations were conducted in a laboratory environment at or around +25° Celsius, using test equipment calibrated against national and/or international standards.

PIM equipment calibration and measurements are conducted in accordance with IEC62037. Kaelus is an ISO9001 certified company and all documentation complies with this standard


Please refer to the product datasheet for the product specifications.

Issued By: Technical Supervisor
Approved By: Quality Manager

Start 824.00 Freq in MHz

Receiver Noise Floor 850 Band - RF Off

Stop 849.00 Freq in MHz

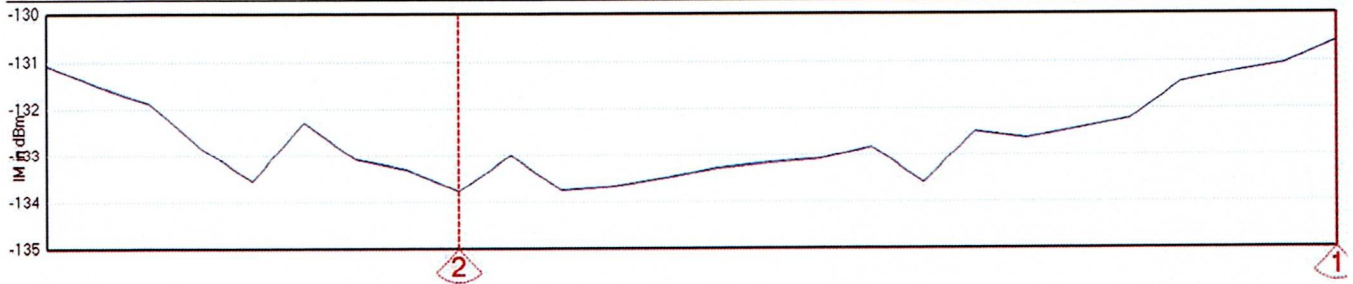


Markers		
No.	Location	Description
1	849 Freq in MHz	Maximum Noise Floor
2	832 Freq in MHz	Minimum Noise Floor

1: Receiver Noise Floor 850 Band - RF Off	
Scale: 1 IM in dBm / Ref: 0 IM in dBm	
Marker.	Measurement
1	-130.59 IM in dBm
2	-133.76 IM in dBm

Start 844.00 Freq in MHz

Swept IM Source 850 Band at 20Watt Tones

Stop 849.00 Freq in MHz

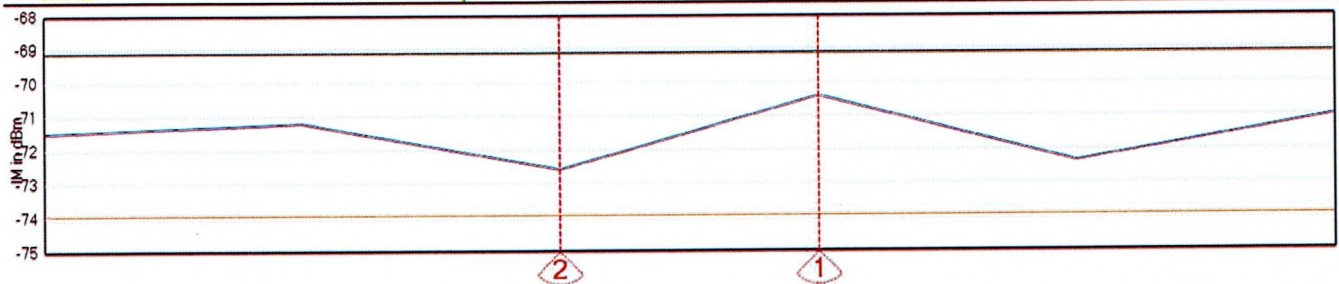

Markers		
No.	Location	Description
1	847 Freq in MHz	Max IM
2	846 Freq in MHz	Min IM

1: Swept IM Source 850 Band at 20Watt Tones	
Scale: 1 IM in dBm / Ref: 0 IM in dBm	
Marker.	Measurement
1	-70.42 IM in dBm
2	-72.59 IM in dBm

2: Upper Limit	
Scale: 1 IM in dBm / Ref: 0 IM in dBm	
Marker.	Measurement
1	-69.12 IM in dBm
2	-69.12 IM in dBm

3: Lower Limit	
Scale: 1 IM in dBm / Ref: 0 IM in dBm	
Marker.	Measurement
1	-73.92 IM in dBm
2	-73.92 IM in dBm

FINAL QUALITY ADMIN TESTS

VALUE UNIT

Calibration Due Date

Apr 4 2024
9:19AM



REPAIR REPORT

Customer Name Entelso Pty Ltd		DATE: 06-April-2023
Customer Reference No. -	Return Authority No. (RMA) BSLMK004295	
Item No. (TypeCode) IPA-0850A	Item Description PORTABLE PIM TESTER	
Original Serial Number	New (current) Serial Number TX2152400189	
Customer Fault Description: Calibration		
Fault Found: Inaccurate Rx readings, damaged battery port on iPA		
Repair Description: Battery port connector replaced. Receiver module reworked. System software updated. Calibration factors updated and tested equipment to ensure all specifications are met.		

Unit passed Final Test:

Unit passed Final QC:

	Name	Department
Reported By:	Mitsu Saka	Customer Service
Authorised By:	Martin Bailey	



Kaelus Pty Ltd – Unit 6 / 29 Smallwood Place, Murarrie, Qld 4172, Australia
Telephone: +61 (0)7 3907 1200 www.kaelus.com ABN: 18 115 398 564