

Certificate of Calibration

INSTRUMENT

Model Number: iPA-1800A
Serial Number: TX2152400196
Description: PORTABLE IM TEST SET-1800MHz iPA-1800A

CERTIFICATION

Calibration Date: April 04 2023
Location of Calibration: 29 Smallwood Place, Murarrie, QLD, 4172, Australia

This document certifies that the instrument detailed above is in conformance with the manufacturer's specifications, which can be accessed on the web address of <http://www.kaelus.com/test-and-measurement-solutions/>.

All calibrations were conducted in a laboratory environment at or around +25° Celsius, using test equipment calibrated against national and/or international standards.

PIM equipment calibration and measurements are conducted in accordance with IEC62037. Kaelus is an ISO9001 certified company and all documentation complies with this standard

Kaelus recommends a calibration interval of 12 months to ensure measurement accuracy. The next recommended calibration date is 04 Apr 2024

Issued By: Technical Supervisor

Approved By: Quality Manager

Customer Test Report

PRODUCT

Model Number : iPA-1800A
Serial Number : TX2152400196
Description : PORTABLE IM TEST SET-1800MHz iPA-1800A

TEST DATA

Verification Date : 03 Apr 2023
Testing Location : 29 Smallwood Place, Murarrie, QLD, 4172, Australia

This document certifies that the instrument detailed above is in conformance with the manufacturer's specifications, which can be accessed on the web address of <http://www.kaelus.com/rf-conditioning-solutions/>.

All calibrations were conducted in a laboratory environment at or around +25° Celsius, using test equipment calibrated against national and/or international standards.

PIM equipment calibration and measurements are conducted in accordance with IEC62037. Kaelus is an ISO9001 certified company and all documentation complies with this standard


Please refer to the product datasheet for the product specifications.

Issued By: Technical Supervisor
Approved By: Quality Manager

Start 1,710.00 Freq in MHz

Receiver Noise Floor DCS-1800 Band - RF Off

Stop 1,785.00 Freq in MHz

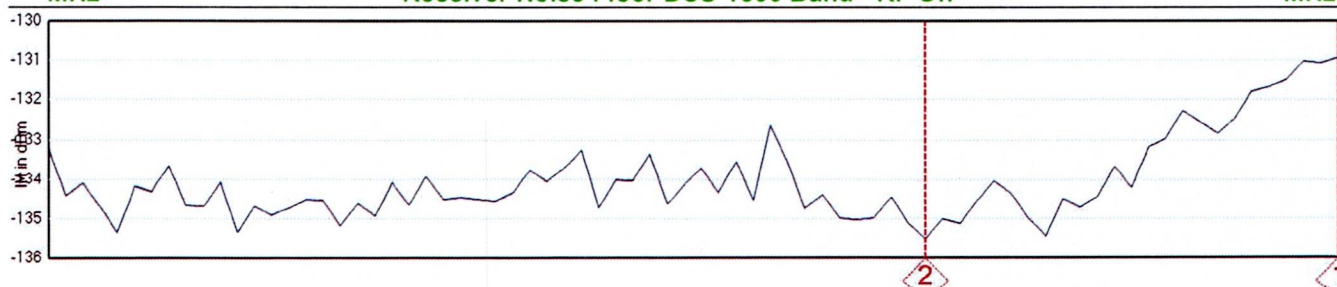

Markers

No.	Location	Description
1	1785 Freq in MHz	Maximum Noise Floor
2	1761 Freq in MHz	Minimum Noise Floor

1: Receiver Noise Floor DCS-1800 Band - RF Off


Scale: 1 IM in dBm / Ref: 0 IM in dBm

Marker.	Measurement
1	-130.91 IM in dBm
2	-135.53 IM in dBm

Start 1,730.00 Freq in MHz

Swept IM Source DCS-1800 Band at 20Watt Tones

Stop 1,785.00 Freq in MHz

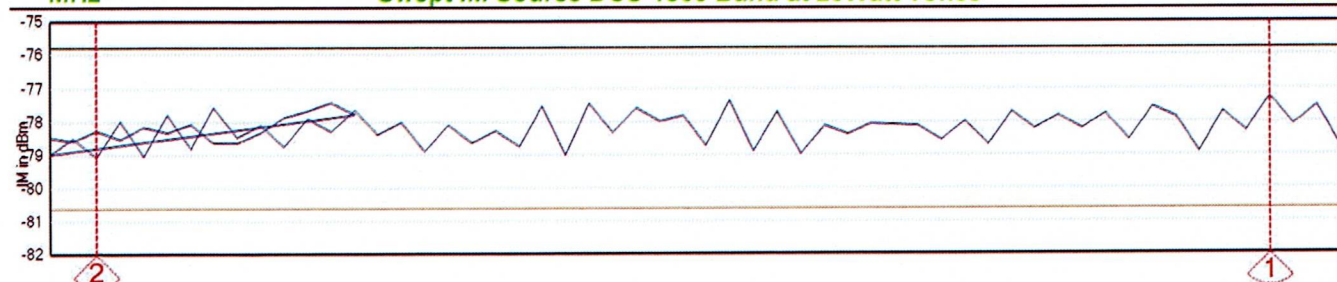

Markers

No.	Location	Description
1	1782 Freq in MHz	Max IM
2	1732 Freq in MHz	Min IM

1: Swept IM Source DCS-1800 Band at 20Watt Tones

Scale: 1 IM in dBm / Ref: 0 IM in dBm

Marker.	Measurement
1	-77.25 IM in dBm
2	-78.27 IM in dBm

2: Upper Limit

Scale: 1 IM in dBm / Ref: 0 IM in dBm

Marker.	Measurement
1	-75.81 IM in dBm
2	-75.81 IM in dBm

3: Lower Limit

Scale: 1 IM in dBm / Ref: 0 IM in dBm

Marker.	Measurement
1	-80.61 IM in dBm
2	-80.61 IM in dBm

FINAL QUALITY ADMIN TESTS

VALUE UNIT

Calibration Due Date

Apr 3 2024
9:04AM



REPAIR REPORT

Customer Name Entelso Pty Ltd		DATE: 06-April-2023
Customer Reference No.	Return Authority No. (RMA) BSLMK004295	
Item No. (TypeCode) IPA-1800A	Item Description PORTABLE PIM TESTER	
Original Serial Number	New (current) Serial Number TX2152400196	
Customer Fault Description: Calibration		
Fault Found: Calibration required		
Repair Description: System software updated. Calibration factors updated and tested equipment to ensure all specifications are met.		

Unit passed Final Test:

Unit passed Final QC:

	Name	Department
Reported By:	Mitsu Saka	Customer Service
Authorised By:	Martin Bailey	



Kaelus Pty Ltd – Unit 6 / 29 Smallwood Place, Murarrie, Qld 4172, Australia
Telephone: +61 (0)7 3907 1200 www.kaelus.com ABN: 18 115 398 564