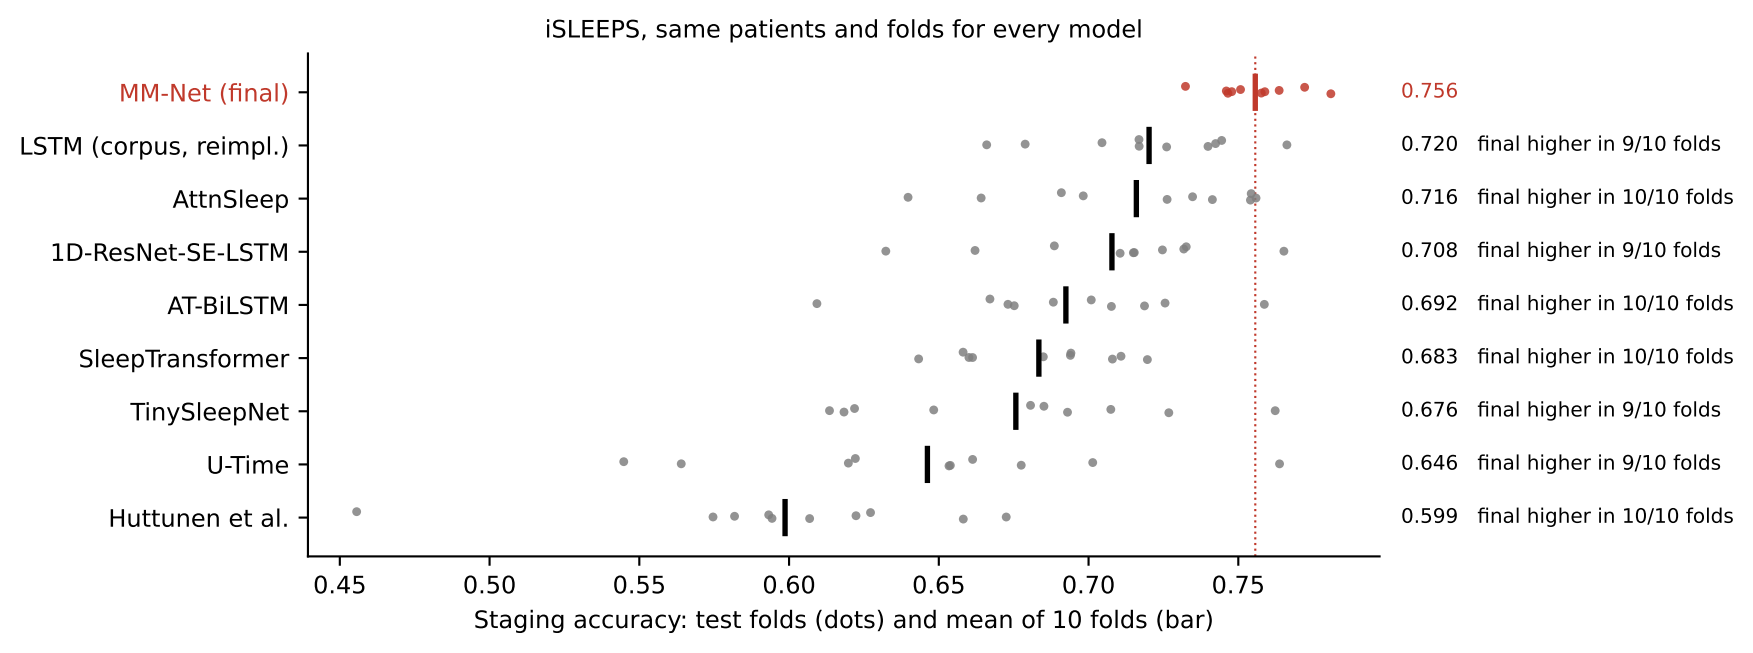
iSLEEPS, same patients and folds for every model
MM-Net (final)
LSTM (corpus, reimpl.)
AttnSleep
1D-ResNet-SE-LSTM
AT-BiLSTM
SleepTransformer
TinySleepNet
U-Time
Huttunen et al.
0.756
0.720 final higher in 9/10 folds
0.716 final higher in 10/10 folds
0.708 final higher in 9/10 folds
0.692 final higher in 10/10 folds
0.683 final higher in 10/10 folds
0.676 final higher in 9/10 folds
0.646 final higher in 9/10 folds
0.599 final higher in 10/10 folds
0.45
0.50
0.55
0.60
0.65
0.70
0.75
Staging accuracy: test folds (dots) and mean of 10 folds (bar)