MM-Net: joint sleep staging and respiratory-event detection after ischemic stroke

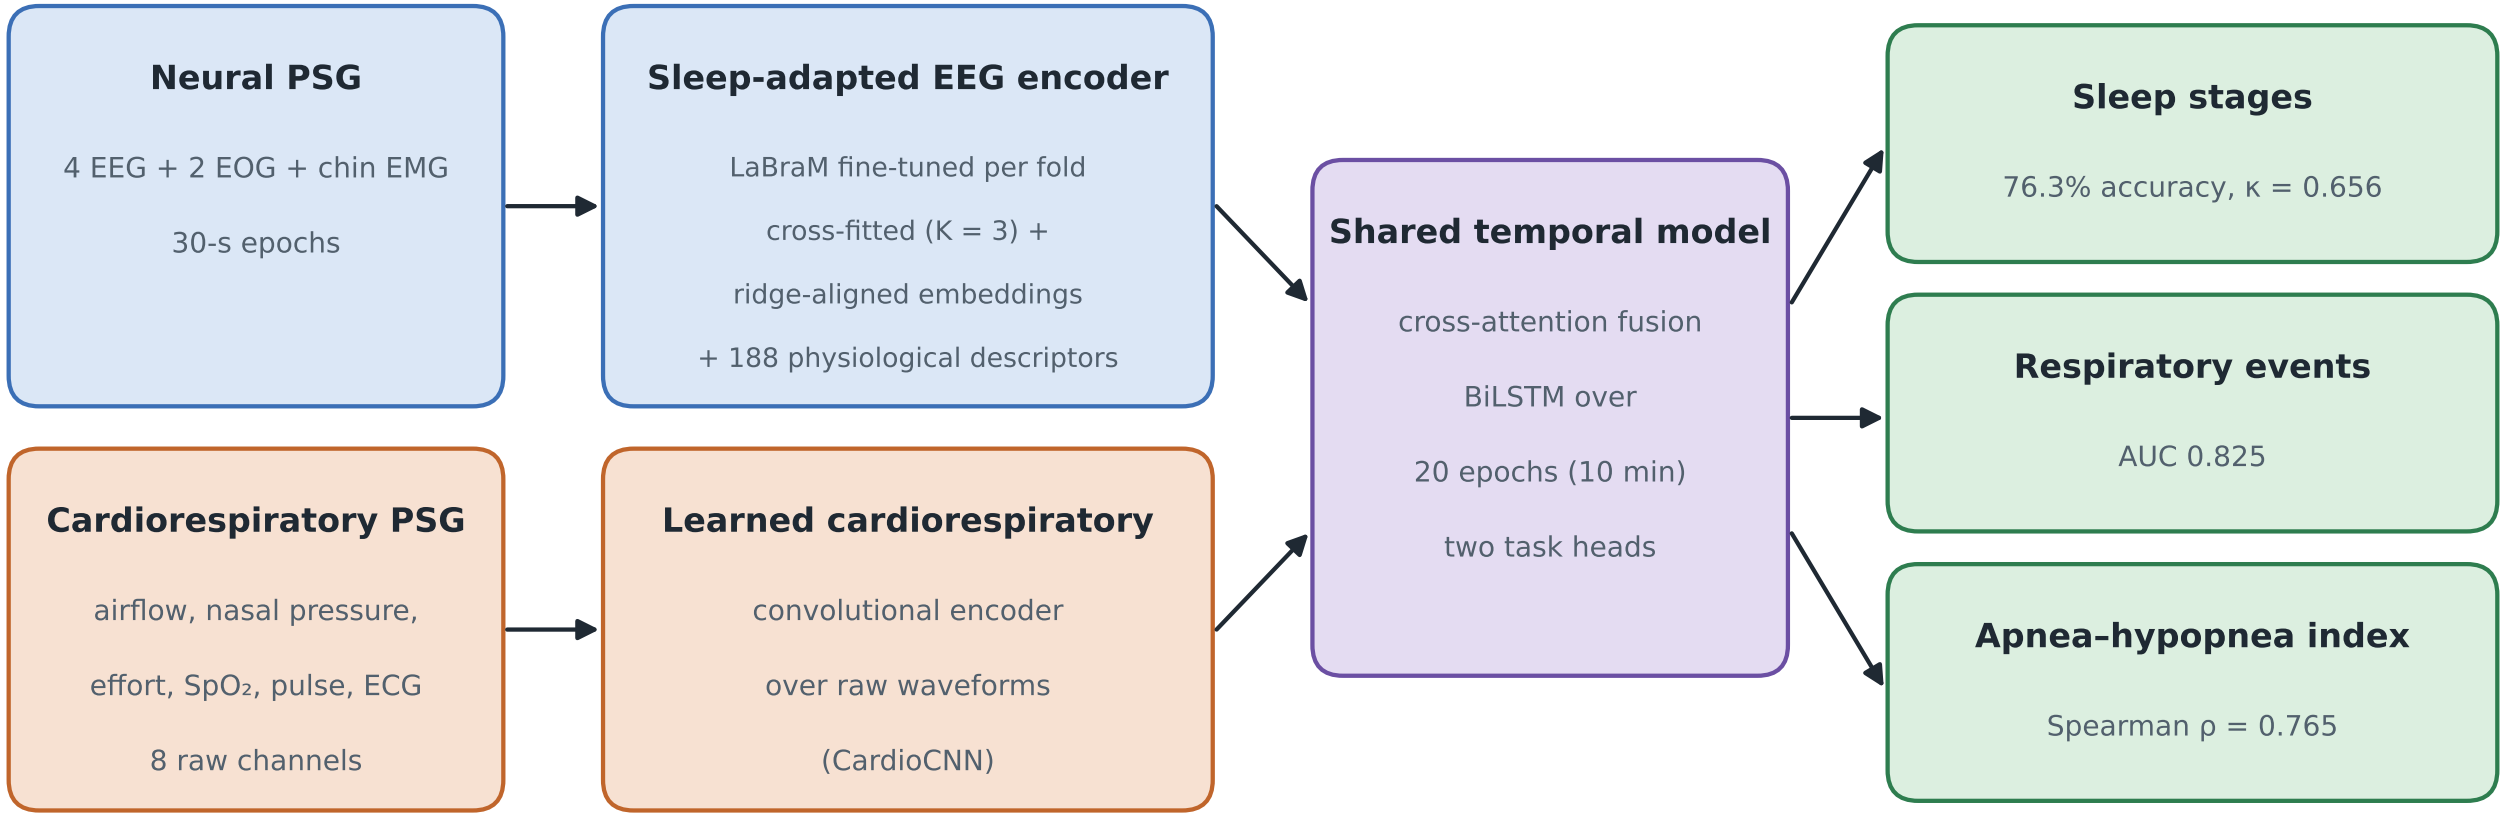

iSLEEPS, 99 patients with subacute ischemic stroke, ten-fold patient-independent evaluation • ISRUC-I: 80.3% accuracy, AUC 0.889 • without retraining: AUC 0.833 (ISRUC-I), 0.841 (UCD)