


DPG10 Power Choke Tester

D.U.T.: DM inductor-non coupled
 Inspector:
 Date: 3/24/2026 3:21:52 PM
 Parameters: 45 A / 10 V / 1000 (491) μ s
 Resistance: 16.73 mOhm

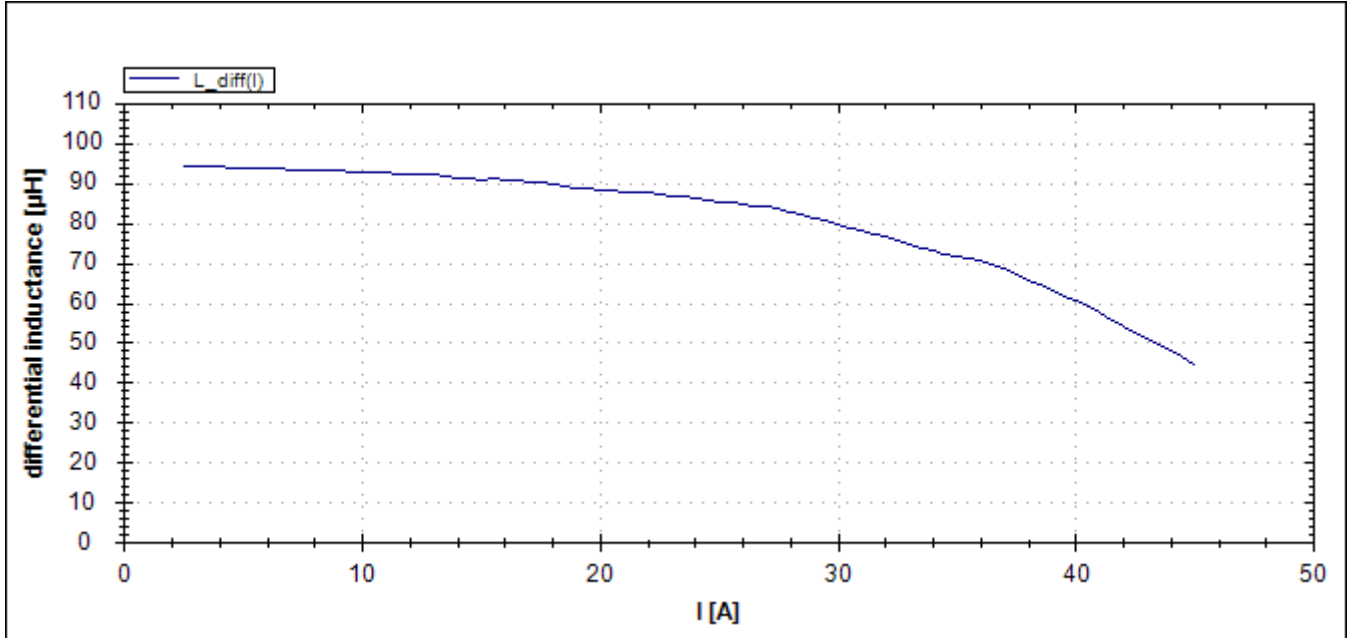

Current [A]	L_diff [μH]	Current [A]	L_diff [μH]	Current [A]	L_diff [μH]	Current [A]	L_diff [μH]	Current [A]	L_diff [μH]
		10.5	92.5	20.5	87.9	30.5	78.8	40.5	58.8
		11.0	92.5	21.0	87.9	31.0	77.9	41.0	57.3
		11.5	92.4	21.5	87.7	31.5	77.1	41.5	55.5
		12.0	92.4	22.0	87.6	32.0	76.3	42.0	54.0
2.5	94.3	12.5	92.3	22.5	87.2	32.5	75.4	42.5	52.6
3.0	94.3	13.0	92.0	23.0	86.8	33.0	74.6	43.0	51.1
3.5	94.2	13.5	91.6	23.5	86.4	33.5	73.7	43.5	49.7
4.0	94.0	14.0	91.4	24.0	86.0	34.0	72.9	44.0	48.1
4.5	93.8	14.5	91.1	24.5	85.6	34.5	72.3	44.5	46.4
5.0	93.8	15.0	90.8	25.0	85.3	35.0	71.7	45.0	44.7
5.5	93.7	15.5	90.9	25.5	85.0	35.5	71.2		
6.0	93.6	16.0	90.7	26.0	84.6	36.0	70.5		
6.5	93.5	16.5	90.4	26.5	84.2	36.5	69.5		
7.0	93.3	17.0	90.3	27.0	83.9	37.0	68.5		
7.5	93.2	17.5	89.9	27.5	83.4	37.5	67.2		
8.0	93.1	18.0	89.6	28.0	82.8	38.0	65.7		
8.5	93.1	18.5	89.1	28.5	82.2	38.5	64.4		
9.0	92.9	19.0	88.8	29.0	81.3	39.0	63.1		
9.5	92.8	19.5	88.5	29.5	80.5	39.5	61.7		
10.0	92.6	20.0	88.2	30.0	79.6	40.0	60.3		